

Guadalupe-Blanco River Authority FY 2026–2027 Clean Rivers Program Quality Assurance Project Plan

***933 E. Court Street
Seguin, Texas 78155***

**Clean Rivers Program
Water Quality Planning Division
Texas Commission on Environmental Quality
P.O. Box 13087, MC 234
Austin, Texas 78711-3087
Effective Period: FY 2026 to FY 2027**


Questions concerning this QAPP should be directed to:

**Elizabeth Malloy (Guadalupe-Blanco River Authority)
GBRA Quality Assurance Officer (QAO)
933 E. Court St.
Seguin, Texas 78155
(830) 305-1056
emalloy@gbra.org**

A2 Approval Page


Texas Commission on Environmental Quality

Water Quality Planning Division




Jason Godeaux, Manager
Water Quality Monitoring and Assessment
Section

8/28/2025
Date



Sarah Whitley, Team Leader
Water Quality Standards and Clean Rivers Program

8/27/2025
Date



Sunshyne Hendrix
Project Quality Assurance Specialist
Clean Rivers Program

8/27/2025
Date



Katrina Smith, Project Manager
Clean Rivers Program


8/26/2025
Date



For Cathy Anderson
Cathy Anderson, Team Leader
Data Management and Analysis

8/28/2025
Date

Air Monitoring Division



D. Jody Koehler,
TCEQ Quality Assurance Manager
Laboratory and Quality Assurance Section

09/02/2025
Date



Loren Walker,
Lead CRP Quality Assurance Specialist
Quality Assurance Team

09/02/2025
Date


Guadalupe-Blanco River Authority



08/20/2025

Elizabeth Edgerton
GBRA CRP Project Manager

Date



8/14/2025

Elizabeth Malloy
GBRA Field Technician, Quality Assurance Officer,
and Backup Data Manager

Date



8/21/2025

Natalie Hickman
GBRA Field Technician and Data Manager

Date



08/21/2025

Lee Gudgell
GBRA Backup Data Manager

Date



8/15/2025

Jack Frank
GBRA Field Technician and Backup Data Manager

Date

Guadalupe-Blanco River Authority (GBRA) Laboratory



08/14/2025

Miliana Hernandez
GBRA Laboratory Director

Date




08/21/2025


Kyle Gudgell
Laboratory Quality Assurance Officer

Date


Upper Guadalupe River Authority (UGRA)



Shelby Taber Date 8/15/2025
UGRA CRP Project Manager, Quality Assurance
Officer, and Data Manager



Travis Linscomb Date 8/15/2025
UGRA Field Technician and Backup Data Manager



Nicole Shepherd Date 8/15/2025
UGRA Laboratory Director and Laboratory Quality
Assurance Officer



Tara Bushnoe Date 8/15/2025
UGRA Backup Data Manager

Hays County (HZ)

Jenna Walker

8.15.25

Jenna Walker
HZ CRP Project Manager

Date

J. Rosenthal

8.15.2025

Jonas Rosenthal
HZ CRP Field Technician

Date

Nicky Vermeersch

Nicky Vermeersch (Aug 15, 2025 11:39:27 CDT)

8.15.2025

Nicky Vermeersch
HZ CRP Quality Assurance Officer

Date

Adam Berglund

8.15.2025

Adam Berglund
HZ CRP Acting Field Technician

Date

The Meadows Center for Water and the Environment (MCWE)

Jenna Walker

8.15.25

Jenna Walker
MCWE CRP Project Manager

Date

Nicky Vermeersch

8.15.2025

Nicky Vermeersch (Aug 15, 2025 11:39:27 CDT)

Nicky Vermeersch
MCWE CRP Quality Assurance Officer

Date


Adam Berglund

8.15.2025

Adam Berglund
MCWE CRP acting Field Technician

Date

SPL, Inc – Kilgore Corporation Environmental Laboratory (SPL)



08/26/2025
Date
William Peery
SPL Laboratory Director



08/26/2025
Date
Kathryn Elliott
SPL Quality Manager

**San Antonio River Authority – Regional Environmental Laboratory
(SARA-REL)**

Zachary Jendrusch 8/15/2025

Zachary Jendrusch Date
SARA Laboratory Director

Jeanette Hernandez 8/15/2025

Jeanette Hernandez Date
SARA Laboratory Quality Assurance Officer

A3 Table of Contents

Guadalupe-Blanco River Authority FY 2026–2027 Clean Rivers Program Quality Assurance Project Plan.....1

A2 Approval Page..... 2

 Texas Commission on Environmental Quality..... 2

 Water Quality Planning Division..... 2

 Air Monitoring Division 2

 Guadalupe-Blanco River Authority..... 3

 Guadalupe-Blanco River Authority (GBRA) Laboratory 3

 Upper Guadalupe River Authority (UGRA) 4

 Hays County (HZ) 5

 The Meadows Center for Water and the Environment (MCWE)..... 6

 SPL, Inc – Kilgore Corporation Environmental Laboratory (SPL)..... 7

 San Antonio River Authority – Regional Environmental Laboratory (SARA-REL)..... 8

A3 Table of Contents..... 9

List of Acronyms 11

A4 Problem Definition/Background.....13

A5 Project/Task Description13

 Amendments to the QAPP14

 Special Project Appendices.....14

A6 Quality Objectives and Criteria.....15

 Ambient Water Reporting Limits (AWRLs)15

 Precision16

 Bias16

 Representativeness16

 Comparability.....16

 Completeness16

A7 Distribution List17

A8 Project/Task Organization21

 Description of Responsibilities21

 TCEQ21

 Guadalupe-Blanco River Authority 22

 Upper Guadalupe River Authority 24

 Meadows Center for Water and the Environment..... 26

 Hays County..... 26

 SPL, Inc – Kilgore Corporation Environmental Laboratory..... 27

 San Antonio River Authority – Regional Environmental Laboratory 27

A9 Project QAM Independence.....28

A10 Project Organizational Chart and Communication 29

 Project Organization Chart..... 29

 Figure A10.1. Organization Chart with Lines of Communication..... 29

A11 Special Training/Certification 30

A12 Documents and Records 30

 Table A12.1 Project Documents and Records31

 Laboratory Test Reports..... 32

 Electronic Data..... 32

B1 Sampling Process Design 33

B2 Sampling Methods..... 33

 Field Sampling Procedures..... 33

 Table B2.1 GBRA, HZ, & MCWE Sample Storage, Preservation, and Handling Requirements 33

 Table B2.2 UGRA Sample Storage, Preservation and Handling Requirements 34

 Sample Containers 35

 GBRA..... 35

 HZ & MCWE 35

 UGRA 36

 Processes to Prevent Contamination 36

	Documentation of Field Sampling Activities.....	36
	Recording Data	37
	Sampling Method Requirements or Sampling Process Design Deficiencies, and Corrective Action	37
	Analytical Methods	38
	Standards Traceability	38
	Analytical Method Deficiencies and Corrective Actions	38
	Acquired Data.....	38
B3	Sample Handling and Custody	39
	Sample Tracking	39
	Sample Labeling.....	39
	Sample Handling	39
	Sample Tracking Procedure Deficiencies and Corrective Action	39
B4	Quality Control	40
	Sampling Quality Control Requirements and Acceptability Criteria.....	40
	Laboratory Measurement Quality Control Requirements and Acceptability Criteria	40
	Quality Control or Acceptability Requirements, Deficiencies, and Corrective Actions	43
B5	Instrument/Equipment Calibration, Testing, Inspection, and Maintenance.....	43
	Instrument Calibration and Frequency	44
B6	Inspection/Acceptance of Supplies and Consumables.....	44
B7	Data Management	44
	Data Management Process	44
	UGRA Data Management Process	45
	HZ and MCWE Data Management Process	46
	Data Errors and Loss	47
	Record Keeping and Data Storage	48
	Data Handling, Hardware, and Software Requirements.....	48
	Information Resource Management Requirements	48
C1	Assessments and Response Actions	49
	Table C1.1 Assessments and Response Requirements	49
	Corrective Action Process for Deficiencies	49
	Corrective Action	50
	Figure C1.1 Corrective Action Process for Deficiencies	51
C2	Reports to Management.....	52
	Table C2.1 QA Management Reports	52
	Reports to GBRA Project Management	52
	Reports to TCEQ Project Management	53
	Reports by TCEQ Project Management	53
D1	Data Review, Verification, and Validation	53
	Verification and Validation Methods.....	53
	Table D1.1: GBRA Data Review Tasks	55
	Table D1.2: UGRA Data Review Tasks.....	57
	Table D1.3: HZ Data Review Tasks	59
	Table D1.4: MCWE Data Review Tasks	61
D2	Reconciliation with User Requirements	63
	Appendix A: Measurement Performance Specifications (Table A6.1a–4d)	64
	Appendix B: Task 3 Work Plan & Sampling Process Design and Monitoring Schedule (Plan)	90
	Sample Design Rationale FY 2026	91
	Site Selection Criteria.....	92
	Monitoring Sites for FY 2026	93
	Appendix C: Station Location Maps	105
	Station Location Maps	105
	Appendix D: Field Data Sheets.....	109
	Appendix E: Chain of Custody Forms.....	116
	Appendix F: Data Review Checklist and Summary Shells.....	120
	Appendix G: Biological Monitoring Electronic Field Sheet	122

List of Acronyms

ALM	Aquatic Life Monitoring
AWRL	Ambient Water Reporting Limit
BMP	Best Management Practices
CAP	Corrective Action Plan
CE	Collecting Entity
CFR	Code of Federal Regulations
COC	Chain of Custody
CRP	Clean Rivers Program
DM	Data Manager
DMRG	Surface Water Quality Monitoring Data Management Reference Guide
DM&A	Data Management and Analysis
EPA	United States Environmental Protection Agency
FY	Fiscal Year
GBRA	Guadalupe-Blanco River Authority
GPS	Global Positioning System
HZ	Hays County
IBWC	International Boundary and Water Commission
LCS	Laboratory Control Sample
LCSD	Laboratory Control Sample Duplicate
LIMS	Laboratory Information Management System
LOD	Limit of Detection
LOQ	Limit of Quantitation
MCWE	Meadows Center for Water and the Environment
MT	Monitoring Type
MS	Matrix Spike
MSD	Matrix Spike Duplicate
NELAC	National Environmental Laboratories Accreditation Conference
NELAP	National Environmental Laboratory Accreditation Program
PM	Project Manager
QA	Quality Assurance
QAM	Quality Assurance Manager
QAO	Quality Assurance Officer
QAPP	Quality Assurance Project Plan
QAS	Quality Assurance Specialist
QC	Quality Control
QM	Quality Manual
QMP	Quality Management Plan
RPD	Relative Percent Difference
RT	Routine Monitoring
SARA-REL	San Antonio River Authority – Regional Environmental Laboratory
SE	Submitting Entity
SLOC	Station Location
SOP	Standard Operating Procedure
SWQM	Surface Water Quality Monitoring
SWQMIS	Surface Water Quality Monitoring Information System
TAC	Texas Administrative Code
TCEQ	Texas Commission on Environmental Quality
TMDL	Total Maximum Daily Load
TNI	The NELAC Institute
TSWQS	Texas Surface Water Quality Standards
TWDB	Texas Water Development Board
UGRA	Upper Guadalupe River Authority
USACE	United States Army Corps of Engineers
VOA	Volatile Organic Analytes

WQS

Water Quality Standard

A4 Problem Definition/Background

In 1991, the Texas Legislature passed the Texas Clean River Act (Senate Bill 818) in response to growing concerns that water resource issues were not being pursued in an integrated, systematic manner. The act requires that ongoing water quality assessments be conducted for each river basin in Texas, an approach that integrates water quality issues within the watershed. The Clean Rivers Program (CRP) legislation mandates that each river authority (or local governing entity) shall submit quality-assured data collected in the river basin to the commission. Quality-assured data in the context of the legislation means data that comply with Texas Commission on Environmental Quality (TCEQ) rules for surface water quality monitoring (SWQM) programs, including rules governing the methods under which water samples are collected and analyzed and data from those samples are assessed and maintained. This QAPP addresses the program developed between the Guadalupe-Blanco River Authority (GBRA) and the TCEQ to carry out the activities mandated by the legislation. The QAPP was developed and will be implemented in accordance with provisions of the TCEQ Quality Management Plan (QMP), Revision 30 or most recent version.

The purpose of this QAPP is to clearly delineate GBRA Quality Assurance (QA) policy, management structure, and procedures which will be used to implement the QA requirements necessary to verify and validate the surface water quality data collected. The QAPP is reviewed by the TCEQ to help ensure that data generated for the purposes described above are of known and documented quality and deemed acceptable for their intended use. This process will ensure that data collected under this QAPP and submitted to the Surface Water Quality Monitoring Information System (SWQMIS) have been collected and managed in a way that guarantees its reliability and therefore can be used in water quality assessments, total maximum daily load (TMDL) projects, water quality standards development, permit decisions, and other program activities deemed appropriate by the TCEQ. Project results will be used to support the achievement of CRP objectives, as contained in the *Guidance for Partners in the Texas Clean Rivers Program FY 2026–2027*.

GBRA in conjunction with UGRA have been monitoring water quality since the mid-1980s and have been actively involved in water quality planning since the early 1970s. By implementing TCEQ's Surface Water Quality Monitoring Program through the Clean Rivers Program, the river authorities have enhanced and modified their existing programs. The expansion of existing monitoring efforts has allowed the river authorities to gather data to characterize water quality conditions in areas not previously monitored. The monitoring goals for the CRP program in the Guadalupe River Basin are to verify the overall health of water bodies evaluated and identify water quality issues. UGRA has been a long-term participant in the Clean Rivers Program data collection efforts. These efforts ensure that TCEQ maintains a consistent historic record of water quality for the Upper Guadalupe River. This long-term water quality dataset allows the river authorities to identify any threats to water quality or degradation in the health of the waterway.

Hays County is a monitoring entity in the Guadalupe River Basin that will coordinate with the Meadows Center to collect data under the GBRA CRP QAPP starting in 2025. Hays County currently funds the Blanco/Cypress Creek Water Quality Monitoring Program, with additional matching funds from Wimberley, Woodcreek, and the Watershed Association. The purpose of this program is to protect regional water resources proactively. The objectives of the monitoring program are to detect and describe spatial and temporal changes, determine impacts of point and nonpoint sources, and assess compliance with established water quality standards for the Blanco River and Cypress Creek. The HZ will collect data at 10 sites on the Blanco River and Cypress Creek quarterly and 3 sites on the Blanco River monthly. These sites are coordinated with the GBRA and TCEQ monitoring schedule annually.

The Meadows Center for Water and The Environment has been monitoring under the GBRA QAPP since 2020. MCWE is a part of the Texas State University System and is focused on environmental issues related to water quantity and quality. They monitor along Cypress Creek and their sites are coordinated with the GBRA and TCEQ monitoring schedule annually.

A5 Project/Task Description

The locations of monitoring sites and scheduled parameters are determined at the Guadalupe River Basin Coordinated Monitoring Meeting. Entities that collect water quality data on the Guadalupe River and its

tributaries attend the coordinated monitoring meeting annually. The collecting entity associated with each monitoring site on the statewide coordinated monitoring schedule is responsible for sample collection and data maintenance at the specified site. The respective collecting entities selected sites for routine monitoring, biological assessment, and diurnal data collection based on stakeholder input, TCEQ assessment needs, budgetary considerations, data gaps, and support of ongoing collection efforts. Each entity collects conventional samples on a monthly or quarterly basis, as specified in the coordinated monitoring schedule.

GBRA collects Secchi measurements only at reservoir sites, UGRA only collects Secchi measurements at stations 15111 and 15113, and the HZ and MC collect Secchi measurements at all of their stations. Flow parameters are reported for all routine freshwater stream monitoring sites, including some impounded streams that retain some lotic properties. Instantaneous flow measurements (00061) are obtained at most stream sites concurrent with the collection of water samples either by direct measurement or from a United States Geological Survey (USGS) or LCRA Hydromet gage if one is located within a quarter mile of the sampling station. If a USGS or LCRA Hydromet gage is greater than a quarter mile from the sampling station, instantaneous flow may still be reported from the gage station if no significant contribution or reduction in flow occurs between the gage and the sampling station, determined on a case-by-case basis and in consultation with the TCEQ CRP PM. However, in cases where flow cannot be directly measured or a flow gage may not accurately reflect conditions at the monitoring site due to inflow/reductions, the discharge data from the closest flow gage may be submitted as a flow estimate (74069) along with flow severity (01351). See Table B1.1 for a list of monitoring stations and associated gages. GBRA collects and analyzes ammonia and total Kjeldahl nitrogen (TKN) at all quarterly collection events and bimonthly at all monthly routine monitoring stations. Ammonia nitrogen is analyzed by UGRA at station 15113 and 12678 quarterly, but TKN is collected and analyzed during all routine quarterly collection events. HZ monitors ammonia nitrogen at all routine quarterly collection events, but only monitors TKN at stations 12661, 17528, 12669, 12660, and 12668. See Appendix B for the project-related work plan tasks and schedule of deliverables for a description of work defined in this QAPP.

See Appendix B for the project-related work plan tasks and schedule of deliverables for a description of work defined in this QAPP.

See Appendix B for sampling design and monitoring pertaining to this QAPP.

Amendments to the QAPP

Amendments to the QAPP may be necessary to address incorrectly documented information or to reflect changes in project organization, tasks, schedules, objectives, and methods. Requests for amendments will be directed from the GBRA Project Manager (PM) to the TCEQ CRP PM electronically. GBRA will submit a completed QAPP amendment document, including a justification of the amendment, a table of changes, and all pages, sections, and attachments affected by the amendment. Amendments are effective immediately upon approval by the GBRA PM, the GBRA Quality Assurance Officer (QAO), the TCEQ CRP PM, the TCEQ CRP Lead Quality Assurance Specialist (QAS), the TCEQ CRP Project QAS, the TCEQ CRP Team Leader, the TCEQ Data Management and Analysis (DM&A) Team Leader, and any additional parties affected by the amendment. Amendments are not retroactive. No work shall be implemented without an approved QAPP or amendment prior to the start of work. Any activities under this contract that commence prior to the approval of the governing QA document constitute a deficiency and are subject to corrective action as described in section C1 of this QAPP. Any deviation or deficiency from this QAPP which occurs after the execution of this QAPP will be addressed through a corrective action plan (CAP). An amendment may be a component of a CAP to prevent future recurrence of a deviation.

Amendments will be incorporated into the QAPP by way of attachment and distributed to personnel on the distribution list by the GBRA PM. If adherence letters are required, GBRA will secure an adherence letter from each sub-tier project participant (e.g., subcontractors, sub-participant, or other units of government) affected by the amendment stating the organization's awareness of and commitment to requirements contained in each amendment to the QAPP. GBRA will maintain this documentation as part of the project's QA records and ensure that the documentation is available for review.

Special Project Appendices

Projects requiring QAPP appendices will be planned in consultation with GBRA, the TCEQ CRP PM, and TCEQ technical staff. Appendices will be written in an abbreviated format and will reference the GBRA QAPP where Guadalupe-Blanco River Authority FY 26–27 CRP QAPP

appropriate. Appendices will be approved by the GBRA PM, the GBRA QAO, the GBRA Laboratory (as applicable), the TCEQ CRP PM, the TCEQ CRP Project QAS, the TCEQ Lead QAS, TCEQ CRP Team Leader, the TCEQ DM&A Team Leader, and additional parties affected by the appendix, as appropriate. Copies of approved QAPP appendices will be distributed by GBRA to project participants before data collection activities commence. The GBRA will secure written documentation from each sub-tier project participant (e.g., subcontractors, subparticipants, other units of government) stating the organization's awareness of and commitment to requirements contained in each special project appendix to the QAPP. GBRA will maintain this documentation as part of the project's QA records and ensure that the documentation is available for review.

A6 Quality Objectives and Criteria

The purpose of routine water quality monitoring is to collect surface water quality data that can be used to characterize water quality conditions, identify significant long-term water quality trends, support water quality standards development, support the permitting process, and conduct water quality assessments in accordance with TCEQ's [Guidance for Assessing and Reporting Surface Water Quality in Texas, February 2024](https://www.tceq.texas.gov/downloads/water-quality/assessment/integrated-report-2024/2024-guidance.pdf) or most recent version (<https://www.tceq.texas.gov/downloads/water-quality/assessment/integrated-report-2024/2024-guidance.pdf>). These water quality data, and data collected by other organizations (e.g., United States Geological Survey [USGS], TCEQ, etc.), will be subsequently reconciled for use and assessed by the TCEQ.

GBRA typically changes which sites receive Aquatic Life Monitoring (ALM) events, using a systematic watershed monitoring approach. Systematic watershed monitoring is defined as sampling that is planned for a short duration (1 to 2 years), is designed to screen waters that would not normally be included in the routine monitoring (RT) program, investigates areas of potential concern, and investigates possible sources of water quality impairments or concerns. Due to the limitations regarding these data (e.g., not temporally representative, limited number of samples, biological sampling does not meet the specimen vouchering requirements), the data will be used to determine whether any locations have values exceeding the TCEQ's water quality criteria and/or screening levels (or in some cases values elevated above normal). GBRA will use this information to determine future monitoring priorities. These water quality data and data collected by other organizations (e.g., USGS, TCEQ, etc.), will be subsequently reconciled for use and assessed by the TCEQ.

The measurement performance specifications to support the project purpose for a minimum data set are specified in Appendix A.

Ambient Water Reporting Limits (AWRLs)

For surface water to be evaluated for compliance with Texas Surface Water Quality Standards (TSWQS) and screening levels, data must be reported at or below specified reporting limits. To ensure data are collected at or below these reporting limits, required ambient water reporting limits (AWRLs) have been established. A full listing of AWRLs can be found at <https://www.tceq.texas.gov/assets/public/waterquality/crp/QA/awrlmaster.pdf>.

The limit of quantitation (LOQ) is the minimum reporting limit, concentration, or quantity of a target variable (e.g., target analyte) that can be reported with a specified degree of confidence by the laboratory analyzing the sample. Analytical results shall be reported down to the laboratory's LOQ (i.e., the laboratory's LOQ for a given parameter is its reporting limit) as specified in Appendix A.

The following requirements must be met in order to report results to the CRP:

- The laboratory's LOQ for each analyte must be set at or below the AWRL. It is the responsibility of GBRA to ensure that any laboratories used to generate CRP data have satisfactory LOQs.
- Once the LOQ is established in the QAPP, that is the reporting limit for that parameter until such time as the laboratory amends the QAPP and lists an updated LOQ.
- The laboratory must demonstrate its ability to quantitate at its LOQ for each analyte by running an LOQ check sample for each analytical batch of CRP samples analyzed.
- Under reasonable circumstances (e.g., the use of a subcontracted lab), data may be reported above or below the LOQ stated in this QAPP, so long as the LOQ remains at or below the AWRL stated in this QAPP.

- Measurement performance specifications for LOQ check samples are found in Appendix A.

Laboratory Measurement Quality Control (QC) Requirements and Acceptability Criteria are provided in Section B4.

Precision

Precision is the degree to which a set of observations or measurements of the same property, obtained under similar conditions, conform to themselves. It is a measure of agreement among replicate measurements of the same property, under prescribed similar conditions, and is an indication of random error.

Laboratory precision is assessed by comparing replicate analyses of laboratory control samples (LCS) in the sample matrix (e.g., deionized water, sand, commercially available tissue), matrix spike/matrix spike duplicate (MS/MSD), or sample/duplicate (DUP) pairs, as applicable. Precision results are compared against measurement performance specifications and used during evaluation of analytical performance. Program-defined measurement performance specifications for precision are defined in Appendix A.

Bias

Bias is the systematic or persistent distortion of a measurement process, which causes errors in one direction (i.e., the expected sample measurement is different from the sample's true value). Bias is a statistical measurement of correctness and includes multiple components of systematic error. Bias is determined through the analysis of LCS and LOQ check samples prepared with verified and known amounts of all target analytes in the sample matrix (e.g., deionized water, sand, commercially available tissue) and by calculating percent recovery. Results are compared against measurement performance specifications and used during evaluation of analytical performance. Program-defined measurement performance specifications for bias are specified in Appendix A.

Representativeness

Site selection, the appropriate sampling regime, comparable monitoring and collection methods, and use of only approved analytical methods will assure that the measurement data represents the conditions at the site. Routine data collected under CRP are considered to be spatially and temporally representative of ambient water quality conditions. Water quality data are collected on a routine frequency and are separated by approximately even time intervals. At a minimum, samples are collected over at least two seasons (to include inter-seasonal variation) and over two years (to include inter-year variation) and include some data collected during an index period (March 15–October 15). Although data may be collected during varying regimes of weather and flow, the data sets will not be biased toward unusual conditions of flow, runoff, or season. The goal for meeting maximum representation of the water body will be tempered by funding availability.

Comparability

Confidence in the comparability of routine data sets for this project and for water quality assessments is based on the commitment of project staff to use only approved sampling and analysis methods and QA/QC protocols in accordance with quality system requirements as described in this QAPP and in TCEQ guidance. Comparability is also guaranteed by reporting data in standard units, by using accepted rules for rounding figures, and by reporting data in a standard format as specified in the Data Management Plan in Section B7.

Completeness

The completeness of the data describes how much of the data are available for use compared to the total potential data. Ideally, 100% of the data should be available. However, the possibility of unavailable data due to accidents, insufficient sample volume, broken or lost samples, etc. is to be expected. Therefore, it will be a general goal of the project(s) that 90% data completion is achieved.

A7 Distribution List

Texas Commission on Environmental Quality
P.O. Box 13087
Austin, Texas 78711-3087

Katrina Smith, Project Manager
Clean Rivers Program
MC-234
(512) 239-5656
katrina.smith@tceq.texas.gov

Cathy Anderson, Team Leader
Data Management and Analysis Team
MC-234
(512) 239-1805
cathy.anderson@tceq.texas.gov

Loren Walker, Lead CRP Quality Assurance Specialist
Laboratory and Quality Assurance Section
MC-165
(512) 239-6340
loren.walker@tceq.texas.gov

Guadalupe-Blanco River Authority

933 E. Court St.
Seguin, Texas 78155

Elizabeth Edgerton, GBRA
CRP Project Manager
(830) 560-3948
eedgerton@gbra.org

Elizabeth Malloy, GBRA Field Technician, Quality
Assurance Officer, and Backup Data Manager
(830)-305-1056
emalloy@gbra.org

Miliana Hernandez, GBRA Laboratory Director
(830) 560-3914
mhernandez@gbra.org

Natalie Hickman, GBRA Field
Technician and Data Manager
(830)-327-5754
nhickman@gbra.org

Jack Frank, GBRA Field Technician and Backup
Data Manager
(830) 305-1065
jfrank@gbra.org

Lee Gudgell, GBRA Backup Data Manager
(830) 560-3970
lgudgell@gbra.org

Kylie Gudgell, GBRA Laboratory Quality Assurance
Officer
(830) 379-5822
kgudgell@gbra.org

The Meadows Center for Water and the Environment

211 San Marcos Springs Drive
San Marcos, TX 78666

Jenna Walker, MCWE CRP Project Manager
(512) 245-9148
jj1433@txstate.edu

Nicky Vermeersch,
MCWE CRP Quality Assurance Officer
(512) 245-4476
nickyv@txstate.edu

Adam Berglund
MCWE CRP acting Field Technician
(512) 245-2561
a_b128@txstate.edu

Hays County

712 S Stagecoach Trail
San Marcos, TX 78666

Jenna Walker, HZ CRP Project Manager
(512) 245-9148
jj1433@txstate.edu

Adam Berglund,
HZ CRP acting Field Technician
(512) 245-2561
a_b128@txstate.edu

Nicky Vermeersch,
HZ CRP Quality Assurance Officer
(512) 245-4476
nickyv@txstate.edu

Jonas Rosenthal
HZ CRP Field Technician
(512) 557-5911
Jonas.rosenthal@hayscountytexas.gov

Upper Guadalupe River Authority

125 Lehmann Dr., Suite 100
Kerrville, Texas 78028

Shelby Taber, UGRA CRP Project Manager, Quality Assurance Officer, and Data Manager
(830) 896-5456 x. 227
staber@ugra.org

Travis Linscomb, UGRA Field Technician and Backup Data Manager
(830) 896-5456 x. 225
tlinscomb@ugra.org

Tara Bushnoe, UGRA Backup Data Manager
(830) 896-5456 x. 222
tbushnoe@ugra.org

Nicole Shepherd, UGRA Laboratory Director and Laboratory Quality Assurance Officer
830-896-5456 x.240
nshepherd@ugra.org

SPL, Inc – Kilgore Corporation Environmental Laboratory
2600 Dudley Rd.
Kilgore, TX 75662

Kathryn Elliott, SPL Laboratory Quality Assurance Officer
(903) 984-0551 ext.20035
Kathryn.elliott@spllabs.com

San Antonio River Authority – Regional Environmental Laboratory
600 E. Euclid Ave.
San Antonio, TX, 78212

Zachary Jendrusch, Laboratory Director
(210) 302-3275
zjendrusch@sariverauthority.org

Jeanette Hernandez, Laboratory Quality Assurance Officer
(210) 302-3283
jhernandez@sariverauthority.org

The TCEQ CRP PM will provide the approved QAPP and any amendments and appendices to TCEQ staff listed in A7 and GBRA. GBRA will provide copies of this project plan and any amendments or appendices of this plan to each person on this list and to each sub-tier project participant (e.g., subcontractors, subparticipants, or other units of government). GBRA will document distribution of the plan and any amendments and appendices, maintain this documentation as part of the project's quality assurance records, and ensure the documentation is available for review.

A8 Project/Task Organization

Description of Responsibilities

TCEQ

Jason Godeaux

Manager, Monitoring and Assessment Section

Responsible for oversight of the implementation of CRP QAPPs, directs the day-to-day management of the section.

Sarah Whitley

Team Leader, Water Quality Standards and Clean Rivers Program

Responsible for TCEQ activities supporting the development and implementation of the Texas CRP. Responsible for verifying that the TCEQ QMP is followed by TCEQ CRP staff. Supervises TCEQ CRP staff. Reviews and responds to any deficiencies, corrective actions, or findings related to the area of responsibility. Oversees the development of QA guidance for the CRP. Reviews and approves all QA audits, corrective actions, reports, work plans, contracts, QAPPs, and TCEQ QMP. Enforces corrective action, as required, where QA protocols are not met. Ensures CRP personnel are fully trained.

Sunshyne Hendrix

CRP Project Quality Assurance Specialist

Serves as liaison between CRP management and TCEQ QA management. Participates in the development, approval, implementation, and maintenance of written QA standards (e.g., Program Guidance, SOPs, QAPPs, QMP). Serves on planning team for CRP special projects. Reviews and approves CRP QAPPs in coordination with other CRP staff. Coordinates documentation and monitors implementation of corrective actions for the CRP.

Katrina Smith

CRP Project Manager

Responsible for the development, implementation, and maintenance of CRP contracts. Tracks, reviews, and approves deliverables. Participates in the development, approval, implementation, and maintenance of written QA standards (e.g., Program Guidance, SOPs, QAPPs, QMP). Coordinates the review and approval of CRP QAPPs in coordination with the TCEQ CRP Project QAS. Ensures maintenance of QAPPs. Assists TCEQ CRP Lead QAS in conducting Basin Planning Agency audits. Verifies QAPPs are being followed by contractors and that projects are producing data of known quality. Coordinates project planning with the Basin Planning Agency PM. Reviews and approves data and reports produced by contractors. Notifies TCEQ CRP QA Specialists of circumstances that may adversely affect the quality of data derived from the collection and analysis of samples. Develops, enforces, and monitors corrective action measures to ensure contractors meet deadlines and scheduled commitments.

Cathy Anderson

Team Leader, Data Management and Analysis Team

Participates in the development, approval, implementation, and maintenance of written QA standards (e.g., Program Guidance, SOPs, QAPPs, QMP). Ensures DM&A staff perform data management-related tasks.

Scott Delgado

CRP Data Manager, Data Management and Analysis Team

Responsible for coordination and tracking of CRP data sets from initial submittal through TCEQ CRP PM review and approval. Ensures that data are reported following instructions in the Data Management Reference Guide (DMRG), July 2019 or most current version. Runs automated data validation checks in SWQMIS and coordinates data verification and error correction with TCEQ CRP PMs. Generates SWQMIS summary reports to

assist CRP PMs' data review. Identifies data anomalies and inconsistencies. Provides training and guidance to CRP and planning agencies on technical data issues to ensure that data are submitted according to documented procedures. Reviews QAPPs for valid stream monitoring stations. Checks validity of parameter codes, submitting entity (SE) code(s), collecting entity (CE) code(s), and monitoring type (MT) code(s). Develops and maintains data management-related SOPs for CRP data management. Coordinates and processes data correction requests. Participates in the development, implementation, and maintenance of written QA standards (e.g., Program Guidance, SOPs, QAPPs, QMP).

D. Jody Koehler

TCEQ Quality Assurance Manager

Responsible for coordinating development and implementation of TCEQ's QA program. Provides oversight and guidance for TCEQ's QA program. Responsible for the development and maintenance of the TCEQ QMP. TCEQ's QA Manager, or designated QA staff in the Laboratory and Quality Assurance Section of the Air Monitoring Division, is responsible for review and approval of program/project QAPPs to ensure QAPPs conform to applicable requirements as detailed in TCEQ's QMP.

Loren Walker

CRP Lead Quality Assurance Specialist

Participates in the development, approval, implementation, and maintenance of written QA standards (e.g., Program Guidance, SOPs, QAPPs, QMP). Assists program manager and TCEQ CRP Project QAS in developing and implementing the quality system. Reviews and approves CRP QAPPs, QAPP amendments, and QAPP special appendices. Prepares and distributes annual audit plans. Conducts monitoring systems audits of planning agencies. Concurs with corrective actions. Conveys QA problems to appropriate management. Recommends that work be stopped in order to safeguard programmatic objectives, worker safety, public health, or environmental protection. Ensures maintenance of audit records for the CRP.

Guadalupe-Blanco River Authority

Elizabeth Edgerton

Guadalupe-Blanco River Authority Project Manager

Responsible for implementing and monitoring CRP requirements in contracts, QAPPs, and QAPP amendments and appendices. Coordinates basin planning activities and work of basin partners. Ensures monitoring systems audits are conducted to ensure QAPPs are followed by basin planning agency participants and that projects are producing data of known quality. Ensures that subparticipants are qualified to perform contracted work. Ensures CRP PMs and/or QA Specialists are notified of deficiencies and corrective actions, and that issues are resolved. Responsible for validating that data collected are acceptable for reporting to TCEQ. The GBRA QAO will assist with completion of the job tasks of the GBRA PM when delegated by the GBRA PM. The GBRA PM will assist with completion of the job tasks of the GBRA QAO, Data Manager (DM), or Field Technician when requested by the primary GBRA QAO/DM/Field Technician.

Elizabeth Malloy

Guadalupe-Blanco River Authority Quality Assurance Officer

Responsible for coordinating the implementation of the QA program. Responsible for writing and maintaining the QAPP and monitoring its implementation. Responsible for maintaining records of QAPP distribution, including appendices and amendments. Responsible for maintaining written records of sub-tier commitment to requirements specified in this QAPP. Responsible for identifying, receiving, and maintaining project QA records. Responsible for coordinating with the TCEQ CRP PM to resolve QA-related issues. Notifies the GBRA PM of particular circumstances which may adversely affect the quality of data. Coordinates and monitors deficiencies and corrective action. Coordinates and maintains records of data verification and validation. Coordinates the research and review of technical QA material and data related to water quality monitoring system design and analytical techniques. Conducts monitoring systems audits on project participants to determine compliance with project and program specifications, issues written reports, and follows through on findings. Ensures that field staff are properly trained and that training records are maintained. The GBRA DM will assist with completion of the job tasks of the GBRA QAO when delegated by the GBRA QAO.

Natalie Hickman

Guadalupe-Blanco River Authority Data Manager

Responsible for ensuring that field data are properly reviewed and verified. Responsible for the transfer of basin quality-assured water quality data to TCEQ in a format compatible with SWQMIS. Maintains quality-assured data on GBRA internet sites.

Natalie Hickman

Guadalupe-Blanco River Authority Field Technician

Performs field data collections for project as specified in Appendix A. Ensures that field staff are properly trained. Notifies the GBRA Laboratory QAO of particular circumstances, which may adversely affect the quality of data. Assists with the preparation of quarterly progress reports to the TCEQ CRP PM. Will assist with UGRA duties when requested.

Elizabeth Malloy

Guadalupe-Blanco River Authority Field Technician

Performs field data collections for project as specified in Appendix A. Ensures that field staff are properly trained. Notifies the GBRA Laboratory QAO of particular circumstances, which may adversely affect the quality of data. Assists with the preparation of quarterly progress reports to the TCEQ CRP PM. Will assist with UGRA duties when requested.

Elizabeth Malloy

Guadalupe-Blanco River Authority Backup Data Manager

Serves as a backup for the duties of the GBRA DM when delegated by the primary DM. The backup DM responsibilities include assisting with the review and verification of laboratory and field data for integrity, continuity, reasonableness and conformance to project requirements, and validation of data against the measurement performance specifications listed in this QAPP. Assists with the transfer of basin quality-assured water quality data to the TCEQ in a format compatible with SWQMIS. Assists with upload of quality-assured data to the GBRA internet sites. The GBRA Backup DM will assist with completion of other job tasks defined in this QAPP as requested by the GBRA PM.

Jack Frank

Guadalupe-Blanco River Authority Field Technician

Performs field data collections for project as specified in Appendix A. Ensures that field staff are properly trained. Notifies the GBRA Laboratory QAO of particular circumstances, which may adversely affect the quality of data. Assists with the preparation of quarterly progress reports to the TCEQ CRP PM. Will assist with UGRA duties when requested.

Jack Frank

Guadalupe-Blanco River Authority Backup Data Manager

Serves as a backup for the duties of the GBRA DM when delegated by the primary DM. The backup DM responsibilities include assisting with the review and verification of laboratory and field data for integrity, continuity, reasonableness and conformance to project requirements, and validation of data against the measurement performance specifications listed in this QAPP. Assists with the transfer of basin quality-assured water quality data to the TCEQ in a format compatible with SWQMIS. Assists with upload of quality-assured data to the GBRA internet sites. The GBRA Backup DM will assist with completion of other job tasks defined in this QAPP as requested by the GBRA PM.

Lee Gudgell

Guadalupe-Blanco River Authority Backup Data Manager

Serves as a backup for the duties of the GBRA DM when delegated by the primary DM. The backup DM responsibilities include assisting with the review and verification of laboratory and field data for integrity, continuity, reasonableness and conformance to project requirements, and validation of data against the measurement performance specifications listed in this QAPP. Assists with the transfer of basin quality-assured water quality data to the TCEQ in a format compatible with SWQMIS. Assists

with upload of quality-assured data to the GBRA internet sites. The GBRA Backup DM will assist with completion of other job tasks defined in this QAPP as requested by the GBRA PM.

Kylie Gudgell

Guadalupe-Blanco River Authority Laboratory Quality Assurance Officer

Responsible for the overall quality control and quality assurance of analyses performed by the GBRA laboratory. Responsible for identifying, receiving, and maintaining project QA records. Notifies the GBRA PM of particular circumstances that may adversely affect the quality of laboratory data. Coordinates and monitors deficiencies and corrective actions associated with laboratory data. Responsible for conducting or hiring an outside party to conduct internal audits annually in compliance with NELAP requirements. The GBRA Laboratory Director will assist with completion of the job tasks of the GBRA Laboratory QAO when requested by the GBRA Laboratory QAO. Ensures that laboratory personnel have adequate training and a thorough knowledge of this QAPP and related SOPs. Ensures that all laboratory data generated for this project has received a review and verification for integrity, continuity, reasonableness and conformance to project requirements.

Miliana Hernandez

Guadalupe-Blanco River Authority Laboratory Director

Responsible for overall performance, administration, and reporting of analyses performed by GBRA Laboratory. Responsible for supervision of laboratory personnel involved in generating analytical data for the project. The responsibilities of the GBRA laboratory Director include supervision of laboratory, purchasing of equipment, and supervision of lab safety program. Trains laboratory analysts to validate data against measurement performance specifications listed in this QAPP. The GBRA Laboratory QAO will assist with completion of the job tasks of the GBRA Laboratory Director when delegated by the GBRA Laboratory Director.

Guadalupe-Blanco River Authority Laboratory Analysts/Technicians

Perform laboratory analysis and assist in collection of field data for project as specified in Appendix A. Notifies the GBRA Laboratory QAO of particular circumstances, which may adversely affect the quality of data. Performs sample custodial duties. Review and verify laboratory data for integrity, continuity, reasonableness and conformance to project requirements, and validates the lab data against the measurement performance specifications listed in this QAPP.

Upper Guadalupe River Authority

Shelby Taber

Upper Guadalupe River Authority Project Manager

Responsible for directing CRP activities in the upper Guadalupe River Basin, in Kerr County, and for one CRP monitoring station in Kendall County. Assures strict compliance with the CRP requirements for project administration and quality assurance. Responsible for coordinating and conducting sampling events, including maintenance of sampling bottles, supplies, and equipment. Maintains records of field data collection and observations. The GBRA PM will assist with completion of the job tasks of the UGRA PM when requested by the UGRA PM. The UGRA Field Technician will assist the UGRA PM with completion of job tasks when delegated.

Shelby Taber

Upper Guadalupe River Authority Quality Assurance Officer

Maintains operating procedures that comply with this QAPP, amendments and appendices. Provides requested information and documentation regarding UGRA monitoring and analysis of CRP data to the GBRA during scheduled monitoring system audits. Ensures that field staff are properly trained and that training records are maintained. Additionally, the UGRA QAO will review and verify all field and laboratory data for integrity and continuity, reasonableness and conformance to project requirements, validating the field and lab data in accordance with the measurement performance

specifications listed in this QAPP. The GBRA QAO will assist with completion of the job tasks of the UGRA QAO when requested by the UGRA PM.

Shelby Taber

Upper Guadalupe River Authority Data Manager

Responsible for ensuring that field and lab data are properly reviewed and verified. Responsible for the transfer of basin quality-assured water quality data to the TCEQ in a format compatible with the DMRG. Maintains link from the water monitoring section of the UGRA web page to the CRP Data Tool web page. The GBRA DM will assist with completion of the job tasks of the UGRA DM when requested by the UGRA PM.

Travis Linscomb

Upper Guadalupe River Authority Field Technician

Performs field data collections for project as specified in Appendix A. Assists the UGRA QAO in ensuring that field staff are properly trained and that training records are maintained. Notifies the UGRA QAO of particular circumstances, which may adversely affect the quality of data. Calibrates and maintains UGRA field instrumentation. Transfers CRP laboratory and field data to an electronic format for review, verification, and validation by the UGRA QAO. The UGRA PM will assist with completion of the job tasks of the UGRA Field Technician when requested by the UGRA Field Technician.

Travis Linscomb

Upper Guadalupe River Authority Backup Data Manager

Serves as a backup for the duties of the UGRA DM when delegated by the primary DM. The backup DM responsibilities include assisting with the review and verification of laboratory and field data for integrity, continuity, reasonableness and conformance to project requirements, and validation of data against the measurement performance specifications listed in this QAPP. Assists with the transfer of basin quality-assured water quality data to the TCEQ in a format compatible with SWQMIS. The UGRA Backup DM will assist with completion of other job tasks defined in this QAPP as requested by the UGRA PM.

Tara Bushnoe

Upper Guadalupe River Authority Backup Data Manager

Serves as a backup for the duties of the UGRA DM when delegated by the primary DM. The backup DM responsibilities include assisting with the review and verification of laboratory and field data for integrity, continuity, reasonableness and conformance to project requirements, and validation of data against the measurement performance specifications listed in this QAPP. Assists with the transfer of basin quality-assured water quality data to the TCEQ in a format compatible with SWQMIS. The UGRA Backup DM will assist with completion of other job tasks defined in this QAPP as requested by the UGRA PM.

Nicole Shepherd

Upper Guadalupe River Authority Laboratory Director and Laboratory Quality Assurance Officer

Responsible for overall performance, administration, quality control, quality assurance, and reporting of analyses performed by UGRA Laboratory. Responsible for supervision of laboratory personnel involved in generating analytical data for the project. Responsible for maintaining quality assurance manual for laboratory operations, maintaining project QA records, and supervision of lab safety program. Ensures that laboratory personnel have adequate training and a thorough knowledge of this QAPP and related SOPs. The lab manager will review and validate all laboratory data for integrity and continuity, reasonableness and conformance to project requirements in accordance with the measurement performance specifications listed in this QAPP. Notifies the UGRA QAO of particular circumstances, which may adversely affect the quality of data. Coordinates and monitors deficiencies and corrective actions associated with laboratory data. Responsible for conducting or hiring an outside party to conduct internal audits annually in compliance with NELAP requirements.

Upper Guadalupe River Authority Laboratory Analysts and Sample Receipt Clerks

Perform laboratory analyses for this project as specified in Appendix A. Notifies the UGRA Laboratory Manager of particular circumstances, which may adversely affect the quality of data. Performs sample custodial duties at time of sample receipt, enters sample information in UGRA LIMS.

Meadows Center for Water and the Environment

Jenna Walker

Meadows Center for Water and the Environment Project Manager

Responsible for directing CRP activities for MCWE. Assures strict compliance with the CRP requirements for project administration and quality assurance.

Nicky Vermeersch

Meadows Center for Water and the Environment Quality Assurance Officer

Maintains operating procedures that comply with this QAPP. Maintains records of field data collection and observations. Responsible for ensuring that data for the MCWE are properly reviewed and verified. Provides information and documentation for partner monitoring systems audits by the GBRA. Responsible for the transfer of MCWE CRP field data to the GBRA PM. Ensures that field staff is properly trained and that training records are maintained.

Adam Berglund

Meadows Center for Water and the Environment Field Technician

Performs field data collections for project as specified in Appendix A. Assists the MCWE QAO in ensuring that field staff are properly trained and that training records are maintained. Notifies the MCWE QAO of particular circumstances, which may adversely affect the quality of data. Calibrates and maintains field instrumentation. Transfers CRP laboratory and field data to an electronic format for review, verification, and validation by the MCWE QAO. Serves as a backup or aid for duties of the HZ field technician when delegated by the HZ field technician in coordination with the HZ PM.

Hays County

Jenna Walker

Hays County Project Manager

Responsible for directing CRP activities for Hays County. Assures strict compliance with the CRP requirements for project administration and quality assurance.

Nicky Vermeersch

Hays County Quality Assurance Officer

Maintains operating procedures that comply with this QAPP. Maintains records of field data collection and observations. Responsible for ensuring that data for the HZ are properly reviewed and verified. Provides information and documentation for partner monitoring systems audits by the GBRA. Responsible for the transfer of HZ CRP field data to the GBRA PM. Ensures that field staff is properly trained and that training records are maintained.

Adam Berglund

Hays County Field Technician

Performs field data collections for project as specified in Appendix A. Assists the HZ QAO in ensuring that field staff are properly trained and that training records are maintained. Notifies the HZ QAO of particular circumstances, which may adversely affect the quality of data. Calibrates and maintains field instrumentation. Transfers CRP laboratory and field data to an electronic format for review, verification, and validation by the HZ QAO. Serves as a backup or aid for duties of the MCWE field technician when delegated by the MCWE field technician in coordination with the HZ PM.

Jonas Rosenthal
Hays County Field Technician

Performs field data collections for project as specified in Appendix A. Assists the HZ QAO in ensuring that field staff are properly trained and that training records are maintained. Notifies the HZ QAO of particular circumstances, which may adversely affect the quality of data. Calibrates and maintains field instrumentation. Transfers CRP laboratory and field data to an electronic format for review, verification, and validation by the HZ QAO. Serves as a backup or aid for duties of the MCWE field technician when delegated by the MCWE field technician in coordination with the HZ PM.

SPL, Inc – Kilgore Corporation Environmental Laboratory

William Peery
SPL Laboratory Director

The responsibilities of the lab director include supervision of laboratory, purchasing of equipment, and supervision of lab safety program. The SPL, Inc – Kilgore lab director will review and verify all laboratory data for integrity and continuity, reasonableness and conformance to project requirements, and then validates against the measurement performance specifications listed in this QAPP.

Kathryn Elliott
SPL Laboratory Quality Assurance Officer

Maintains quality assurance manual for laboratory operations, maintains operating procedures that are in compliance with this QAPP, amendments and appendices. Conducts in-house audits to ensure compliance with written SOPs, NELAP requirements and to identify potential problems. Responsible for the overall quality control and quality assurance of analyses performed by SPL laboratories. Reviews and verifies all laboratory data for integrity and continuity, reasonableness and conformance to project requirements, and then validates against the measurement performance specifications listed in this QAPP.

San Antonio River Authority – Regional Environmental Laboratory

Zachary Jendrusch
San Antonio River Authority Laboratory Director

Responsible for overall performance, administration, and reporting of analyses performed by SARA's Laboratory. Responsible for supervision of laboratory personnel involved in generating analytical data for the project. Ensures that laboratory personnel have adequate training and a thorough knowledge of this QAPP and related SOPs. Responsible for oversight of all laboratory operations ensuring that all QA/QC requirements are met, documentation is complete and adequately maintained, and results are reported accurately. Additionally, the lab director ensures that all laboratory data is reviewed and verified for integrity and continuity, reasonableness and conformance to project requirements, and then validated against the data quality objectives listed in Appendix A of this QAPP.

Jeanette Hernandez
San Antonio River Authority Laboratory Quality Assurance Officer

Maintains quality assurance manual for laboratory operations, maintains operating procedures that are in compliance with this QAPP, amendments and appendices. Conducts in-house audits to ensure compliance with written SOPs, NELAP requirements and to identify potential problems. Responsible for the overall quality control and quality assurance of analyses performed by SARA-REL. Reviews and verifies all laboratory data for integrity and continuity, reasonableness and conformance to project requirements, and then validates against the measurement performance specifications listed in this QAPP.

A9 Project QAM Independence

TCEQ uses a semi-decentralized QA program, which is organizationally independent of operational programs and activities within the agency. TCEQ's QA program has sufficient access and authority to coordinate the development and implementation of the agency's quality system.


The TCEQ QA Manager (QAM) and designated TCEQ QA staff from the Laboratory and Quality Assurance Section within the Air Monitoring Division of the Office of Air are independent of activities performed by CRP. No CRP staff have authority to sign QAPPs, amendments, or appendices on behalf of TCEQ's QAM or the Lead CRP QAS. Similarly, TCEQ's QAM and the Lead CRP QAS cannot sign QAPPs, amendments or appendices on behalf of CRP staff.

Roles of project QA staff are described in Section A8. An illustration of QA independence and lines of communication and supervision for this project are detailed in the project organization chart in A10. Communication for deficiencies and corrective actions are described in Section C1.

A10 Project Organizational Chart and Communication

Project Organization Chart

Figure A10.1. Organization Chart with Lines of Communication

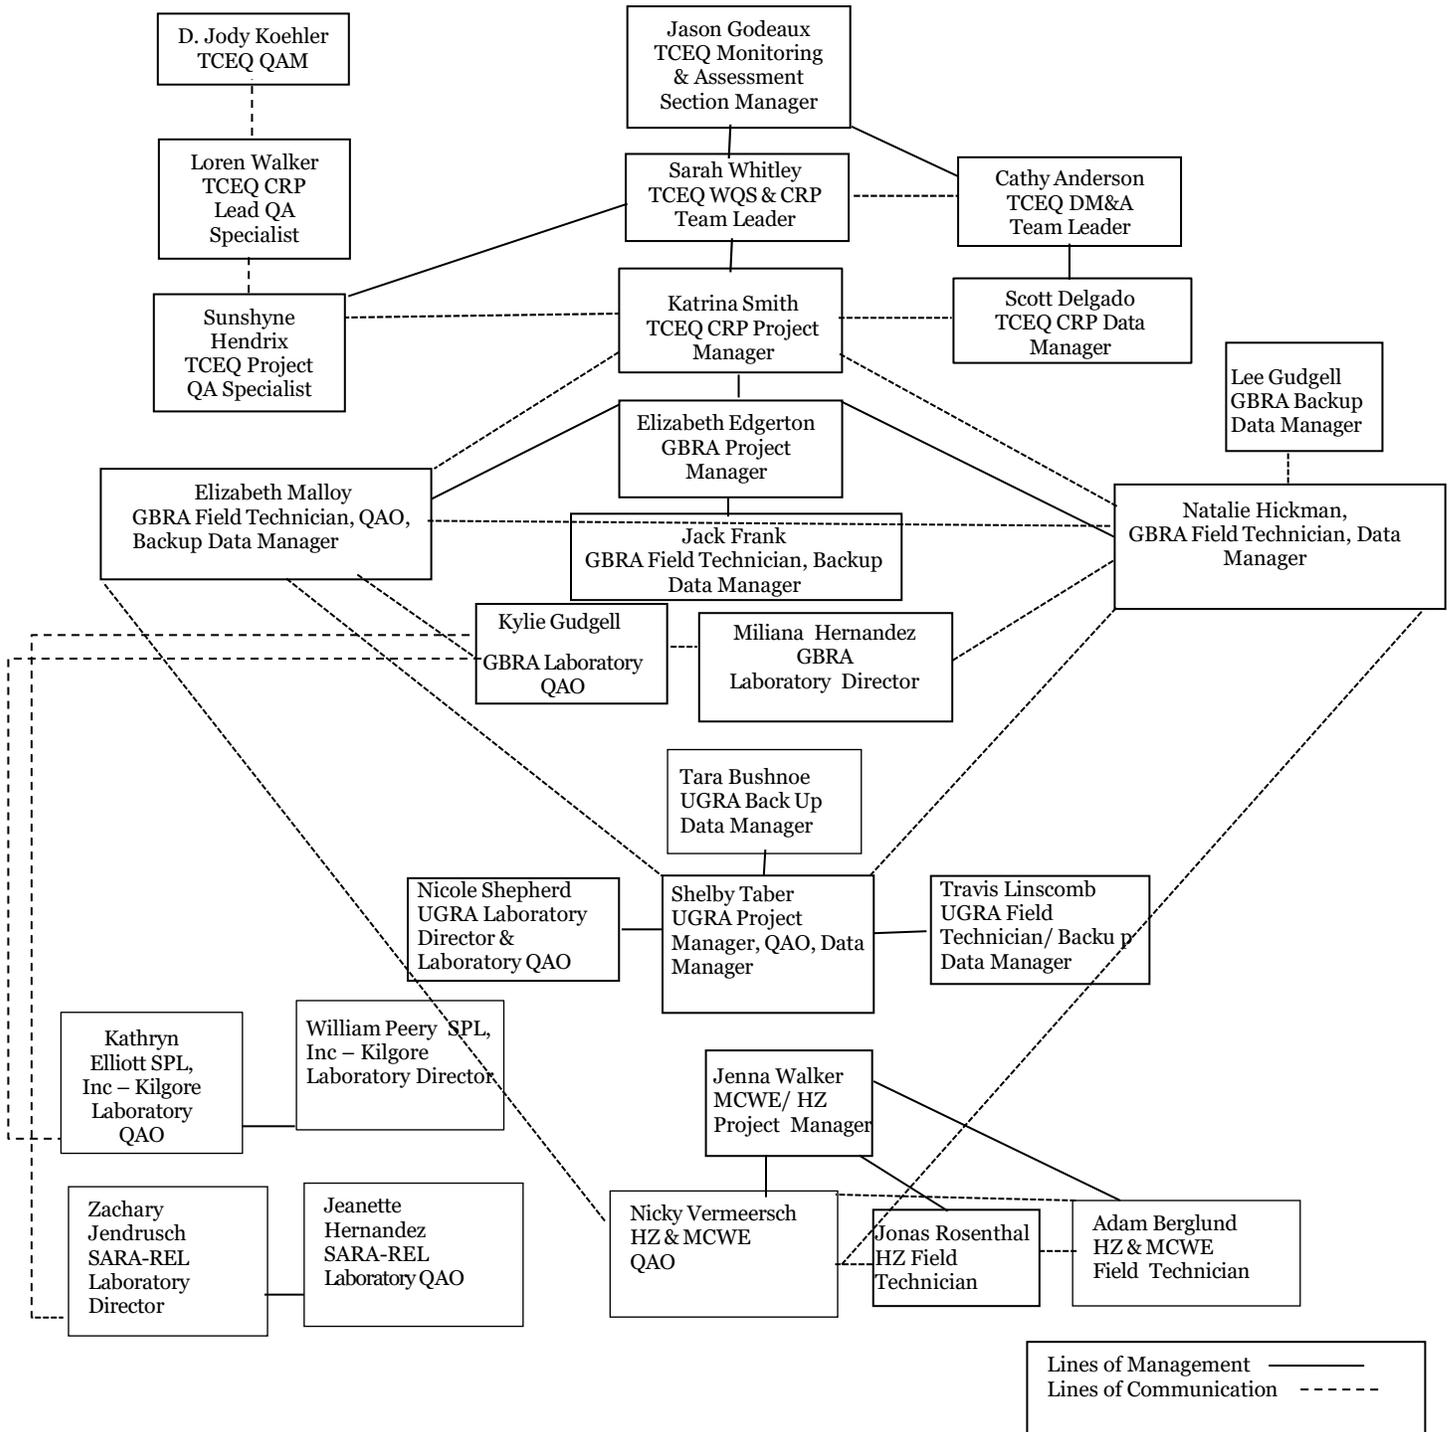

A11 Special Training/Certification

Before new field personnel independently conduct field work, the Field Technicians (or designees) train him/her in proper instrument calibration, field sampling techniques, and field analysis procedures. The GBRA QAO (or designee) will document the successful field demonstration. The GBRA QAO (or designee) will retain documentation of training and the successful field demonstration in an electronic archive and ensure that the documentation will be available during monitoring systems audits. All full-time employees are eligible to be trained to conduct field work independently. Any part-time employees or students who wish to receive this training must get written approval from the GBRA PM.

The requirements for obtaining certified positional data using a global positioning system (GPS) are located in Section B7, Data Management.

Contractors and subcontractors must ensure that laboratories analyzing samples under this QAPP meet the requirements contained in The National Environmental Laboratories Accreditation Conference (NELAC) Institute Standard (2016) Volume 1, Module 2, Section 4.5 (concerning Subcontracting of Environmental Tests).

A12 Documents and Records

The documents and records that describe, specify, report, or certify activities are listed. The list below is limited to documents and records that may be requested for review during a monitoring systems audit. All documents generated by GBRA are saved as electronic copies for retention. If a document cannot be produced electronically, then a paper copy will be created and saved as an electronic copy. Paper files are retained for at least one month after creation and electronic files are retained for at least 5 years. Project documents (e.g., QAPPs, field and laboratory SOPs, copies of laboratory quality manuals, etc.) may be retained up to the period of record of the most recent TCEQ 2024 Integrated Report (e.g. 5 years). GBRA submits the monitoring data collected by the GBRA, HZ and MCWE directly to TCEQ in a format compatible with SWQMIS.

All monitoring analysis data generated by the GBRA laboratory is recorded on electronic bench sheets or in electronic instrument files. The results from these files are transferred into the GBRA Laboratory Information Management System (LIMS) with an electronic parsing program. Electronic bench sheets and instrument files associated with monitoring data are archived for at least 5 years.

GBRA Field Technicians use a computer to record field data and instrument calibration logs onto electronic data sheets. GBRA Field Technicians transfer the data that they record on electronic field sheets into the GBRA laboratory information system (LIMS) with an electronic parsing program. A GBRA Field Technician saves the electronic data sheets associated with monitoring data for at least 5 years. Alternatively, GBRA Field Technicians may record field data and instrument calibrations on paper data sheets. GBRA Field Technician transcribe the data from the paper field sheets into the GBRA LIMS manually. GBRA field technicians retain paper data sheets for at least one month, and then transfers the files to GBRA records retention staff for long term electronic archiving. GBRA Field Technicians will determine the method in which field data is collected based upon electronic equipment availability and access to wireless communications.

The HZ and MCWE Field Technicians record data on a computer into electronic field sheets that they email to the GBRA PM along with associated equipment calibration logs following routine monitoring collection events. The GBRA PM or Field Technician electronically parses the data from these field sheets into the GBRA LIMS. Alternatively, the HZ and MCWE Field Technicians may record field data and instrument calibrations on paper data sheets as a backup if electronic means malfunction or are not available. The HZ and MCWE Field Technicians will determine the method in which field data is collected based upon electronic equipment availability and access to wireless communications.

The GBRA, HZ, and MCWE all save electronic copies of these field sheets and calibration logs as pdfs for at least 5 years. If changes are needed for a file saved as a pdf, the original will not be deleted, but a new pdf will be saved with the same name and the date that it was updated as well as the initials of the person who updated the file.

UGRA maintains all paper and electronic laboratory bench sheets, field sheets, and instrument calibration logs associated with their routine monitoring stations for at least 5 years. UGRA submits the routine monitoring data that they collect directly to TCEQ in a format compatible with SWQMIS. The UGRA Field Technician submits UGRA twenty-four hour diel data associated with GBRA ALM events to GBRA electronically via email in an excel spreadsheet. GBRA transcribes the data from these ALM events into a format compatible with SWQMIS and submits them to TCEQ.

Table A12.1 Project Documents and Records

Document/Record	Location	Retention (yrs)	Format
QAPPs, amendments, and appendices	GBRA/UGRA ¹ /HZ/MCWE/ SPL ⁴ /SARA-REL ⁵	5 years	Electronic ⁶
Field SOPs	GBRA/UGRA ¹ /HZ/MCWE	5 years	Electronic ⁶
Laboratory quality manuals	GBRA/UGRA ¹ / SPL /SARA-REL ⁵	5 years	Electronic ⁶
Laboratory SOPs	GBRA/UGRA ¹ / SPL ⁴ /SARA-REL ⁵	5 years	Electronic ⁶
QAPP distribution documentation	GBRA	5 years	Electronic ⁶
Field staff training records	GBRA ² /UGRA ¹ /MCWE ³ /HZ ³	1 month/ 5 years	Paper/ Electronic
Field equipment calibration/maintenance logs	GBRA ² /UGRA ¹ /HZ ³ /MCWE ³	1 month/ 5 years	Paper/ Electronic
Field instrument printouts	GBRA/UGRA/HZ/MCWE	5 years	Electronic ⁶
Field notebooks or data sheets	GBRA ² /UGRA ¹ /HZ ³ /MCWE ³	1 month/ 5 years	Paper/ Electronic
Chain of custody records	GBRA ² /UGRA ¹ / SPL ⁴ /SARA-REL ⁵	1 month/ 5 years	Paper/ Electronic
Laboratory calibration records	GBRA ² /UGRA ¹ / SPL ⁴ /SARA-REL ⁵	1 month/ 5 years	Paper/ Electronic
Laboratory instrument printouts	GBRA ² /UGRA ¹ / SPL ⁴ /SARA-REL ⁵	1 month/ 5 years	Paper/ Electronic
Laboratory data reports/results	GBRA/UGRA/HZ/MCWE/ SPL ⁴ /SARA-REL ⁵	5 years	Electronic ⁶
Laboratory equipment maintenance logs	GBRA ² /UGRA ¹ / SPL ⁴ /SARA-REL ⁵	1 month/ 5 years	Paper/ Electronic
Corrective action documentation	GBRA ² /UGRA ¹ /HZ/MCWE/ SPL ⁴ /SARA-REL ⁵	1 month/ 5 years	Paper/ Electronic

¹ UGRA maintains all original paper documentation for 5 years from creation.

² GBRA retains copies of all produced paper documents for at least 1 month from creation, at which point a document is scanned and converted to an electronic copy, which is retained by the GBRA for at least 5 years.

³ HZ/MCWE retains copies of all produced paper documents for at least one month. These documents are converted to electronic format and retained for at least five years. Electronically produced field sampling documents are emailed to, and retained by the GBRA for at least 5 years.

⁴ SPL retains all documentation in electronic format. Any generated paper data is converted to electronic format and retained for at least five years.

⁵ SARA-REL retains all documentation in electronic format. Any generated paper data is converted to electronic format and retained for at least five years.

⁶These documents are generated and retained electronically for at least 5 years. If printed paper copies are generated, they are not considered controlled documents.

Laboratory Test Reports

Test/data reports from the laboratory must document the test results clearly and accurately. Routine data reports should be consistent with The NELAC Institute (TNI) Standard (2016), Volume 1, Module 2, Section 5.10 and include the information necessary for the interpretation and validation of data. The requirements for reporting data and the procedures are provided.

The LIMS from each contributing laboratory generates a test report upon request. A laboratory test report will contain at least the following information:

- Title of report and unique identifiers on each page
- Name and address of the analytical laboratory
- Name and customer number of the client
- Identification of the sample(s) analyzed
- Date and time of sample receipt
- Clearly identified subcontracted laboratory results (as applicable)
- Identification of analysis method
- Identification of samples that did not meet QA requirements and why (e.g., holding times exceeded)
- Name and title of person accepting responsibility for the report
- Sample results
- Units of measurement
- Sample matrix
- Dry weight or wet weight (as applicable)
- Station information
- Date and time of collection
- Sample depth
- Holding time for *E. coli*
- LOQ and limit of detection (LOD) (formerly referred to as the reporting limit and the method detection limit, respectively), and qualification of results outside the working range (if applicable)
- Certification of NELAP compliance
- Narrative information on QC failures or deviations from requirements that may affect the quality of results or is necessary for the review, verification and validation of data

The information in test reports should be consistent with the information that the Guadalupe-Blanco River Authority and Upper Guadalupe River Authority need to prepare data submittals to TCEQ.

Otherwise, reports should be consistent with the TNI Standard and should include any additional information critical to the review, verification, validation, and interpretation of data. Information included in reports is based on the process used by the GBRA or UGRA DM and documented in Section D1 and D2 of this document.

The LIMS generates quality assured electronic data for the GBRA or UGRA Data Manager. The GBRA or UGRA DM ensures that a review, verification, and validation of the electronic data has occurred prior to submitting it to TCEQ in a format acceptable by SWQMIS.

Electronic Data

HZ and MCWE send electronic or paper data sheets to GBRA. UGRA directly submits data to TCEQ. Data will be submitted electronically by GBRA and UGRA to TCEQ in the Event/Result file format described in the most current version of the DMRG, which can be found at https://www.tceq.texas.gov/waterquality/datamanagement/dmrg_index.html. A completed Data Review Checklist and Data Summary (see Appendix F) will be included with each data submittal.

B1 Sampling Process Design

See Appendix B for sampling process design information and monitoring tables associated with data collected under this QAPP.

B2 Sampling Methods

Field Sampling Procedures

Field sampling will be conducted in accordance with the latest versions of the *TCEQ Surface Water Quality Monitoring Procedures Volume 1: Physical and Chemical Monitoring Methods, 2012* (RG-415) and *Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014* (RG-416), collectively referred to as “SWQM Procedures.” Updates to SWQM Procedures are posted to the Surface Water Quality Monitoring Procedures website (https://www.tceq.texas.gov/waterquality/monitoring/swqm_guides.html), and shall be incorporated into GBRA, UGRA, HZ, and MCWE’s procedures, QAPP, SOPs, etc., within 60 days of any final published update. Additional aspects outlined in Section B below reflect specific requirements for sampling under CRP and/or provide additional clarification.

Table B2.1 GBRA, HZ, & MCWE Sample Storage, Preservation, and Handling Requirements

Parameter	Matrix	Container	Preservation	Sample Volume	Holding Time
Turbidity***	Surface Water	Plastic	Cool, < 6°C but >0°C	3L	48 Hours
Hardness***	Surface Water	Plastic	Cool, < 6°C but >0°C; H ₂ SO ₄ to pH < 2**	1L	6 Months
Total Suspended Solids (TSS)	Surface Water	Plastic	Cool, < 6°C but >0°C	3L	7 Days
Nitrate-nitrogen	Surface Water	Plastic	Cool, < 6°C but >0°C	3L	48 Hours
Nitrite –***	Surface Water	Plastic	Cool, < 6°C but >0°C	3L	48 Hours
Ammonia-nitrogen	Surface Water	Plastic	Cool, < 6°C but >0°C; H ₂ SO ₄ to pH < 2**	1L	28 Days
Total phosphorus	Surface Water	Plastic	Cool, < 6°C but >0°C; H ₂ SO ₄ to pH < 2**	1L	28 Days
Total Kjeldahl Nitrogen +	Surface Water	Plastic	Cool, < 6°C but >0°C; H ₂ SO ₄ to pH < 2**	1L	28 Days
Sulfate***	Surface Water	Plastic	Cool, < 6°C but >0°C	3L	28 Days
Chloride***	Surface Water	Plastic	Cool, < 6°C but >0°C	3L	28 Days
Chlorophyll a***/ Pheophytin* **	Surface Water	Amber Plastic	Dark, Cool, < 6°C but >0°C before Filtration; Dark, 0°C after Filtration	3L	Filter within 48 Hours; 24 or 28 days at 0°C ****.
<i>E. coli</i>	Surface Water	Plastic (Sterile)	Cool, < 6°C but >0°C ; no preservative (with Na ₂ S ₂ O ₃)	120 mL	8 Hours*

			downstream of chlorinated discharges)**		
Biological*** Fish	Surface Water	Plastic	10% Formalin (field) **/ 70%-75% Ethyl Alcohol (Voucher)	500 mL	1 week (field); 5 years (voucher)
Biological*** Benthic Macro-invertebrates	Surface Water	Plastic	70% - 95% Ethyl Alcohol (field) **/ 70%-75% Ethyl Alcohol (voucher)	500 mL (field) / 5 mL (voucher)	1 week (field); 5 years (voucher)

* *E.coli* samples should always be processed as soon as possible and incubated no later than 8 hours from time of collection. When transport conditions necessitate sample incubation after 8 hours from time of collection, the holding time may be extended and samples must be processed as soon as possible and within 30 hours.

** Preservation occurs within 15 minutes of collection in a pre-preserved bottle.

*** HZ and MCWE do not collect this parameter

**** Maximum holding time is 28 days for method SM10200-H4 or SM10200-H and 24 days if using EPA method 445.0

+ MCWE does not collect this parameter

Table B2.2 UGRA Sample Storage, Preservation and Handling Requirements

Parameter	Matrix	Container	Preservation	Sample Volume	Holding Time
Turbidity	Surface Water	Plastic	Cool, < 6°C but >0°C	1L	48 Hours
Total Suspended Solids (TSS)	Surface Water	Plastic	Cool, < 6°C but >0°C	1L	7 Days
Nitrate-nitrogen	Surface Water	Plastic	Cool, < 6°C but >0°C	1L	48 Hours
Ammonia-nitrogen	Surface Water	Plastic	Cool, < 6°C but >0°C; H ₂ SO ₄ to pH < 2****	250 mL	28 Days
Total phosphorus	Surface Water	Plastic	Freeze without chemical preservation	250 mL	28 Days
Total Kjeldahl Nitrogen	Surface Water	Plastic	Cool, < 6°C but >0°C; H ₂ SO ₄ to pH < 2**	500 mL	28 Days
Sulfate	Surface Water	Plastic	Cool, < 6°C but >0°C	1L	28 Days
Chloride	Surface Water	Plastic	Cool, < 6°C but >0°C	1L	28 Days
Chlorophyll a /Pheophytin	Surface Water	Amber Plastic	Dark, Cool, < 6°C but >0°C before Filtration; Dark, 0°C after Filtration	1L	Filter within 48 Hours; 24 or 28 days at 0°C*****.
<i>E. coli</i>	Surface Water	Plastic (Sterile)	Cool, < 6°C but >0°C; Na ₂ S ₂ O ₃ **	120 mL***	8 Hours*

* *E. coli* samples should always be processed as soon as possible and incubated no later than 8 hours from time of collection. When transport conditions necessitate sample incubation after 8 hours from time of collection, the holding time may be extended and samples must be processed as soon as possible and within 30 hours.

** Preservation occurs within 15 minutes of collection in a pre-preserved bottle.

*** UGRA collects *E. coli* duplicates in 250 mL sterile bottles.

**** Preservation occurs upon arrival at UGRA lab unless analyzed within a 24-hour period.

***** Maximum holding time is 28 days for method SM10200-H4 or SM10200-H and 24 days if using EPA method 445.0

Sample Containers

GBRA

GBRA either purchases new bottles or uses bottles that are cleaned and reused for all samples collected for the Clean Rivers Program.

- For unpreserved conventional parameters such as TSS, Nitrate (NO₃-N), Nitrite (NO₂-N), Turbidity, Chloride, Sulfate, Chlorophyll a, and Pheophytin, GBRA uses three-liter amber bottles that are either purchased new or cleaned and reused. The unpreserved reused bottles are cleaned by GBRA staff with the following procedure: 1) wash containers with tap water and laboratory grade detergent, 2) triple rinse with hot tap water, and 3) triple rinse with deionized water. GBRA will dispose of reused bottles for conventional analysis if the reused bottles visibly appear discolored or are no longer water tight following the cleaning procedure.
- Sample containers for parameters preserved with sulfuric acid (H₂SO₄) such as TKN, Ammonia (NH₃-N), Total Phosphorus and Total Hardness are one-liter plastic bottles pre-preserved with 2 mL of sulfuric acid that GBRA either purchases new or cleans, preserves, and reuses. The reused preserved bottles are cleaned by GBRA staff with the following procedure: 1) wash containers with tap water and laboratory grade detergent, 2) triple rinse with hot tap water, and 3) triple rinse with deionized water. After cleaning, 2 mL of sulfuric acid are added to bottles for sample preservation. GBRA will dispose of reused bottles for conventional analysis if the reused bottles visibly appear discolored or are no longer water tight following the cleaning procedure. GBRA maintains certificates from sample container manufacturers for purchased bottles in a notebook located in the GBRA laboratory.
- Sample containers for bacteria parameters such as *E. coli* are 120 mL sterile bottles. GBRA collects bacteriological samples in bottles without sodium thiosulfate for most monitoring locations. Samples collected immediately downstream of chlorinated discharges are collected in bottles preserved with sodium thiosulfate.
- GBRA takes 2 photo vouchers per species of fish while in the field. If the fish is unable to be identified in the field, GBRA collects sample containers with 10% formalin for biological fish vouchers in the field. These samples are stored for at least 1 week and then washed and soaked in tap water for three successive days. Following this washing procedure, GBRA transfers the fish to bottles containing 70-75% Ethyl Alcohol to serve as vouchers for each fish species collected.
- GBRA collects sample containers with 70-95% Ethyl Alcohol for biological benthic macroinvertebrates assemblages in the field. These samples are stored at room temperature until the sample is processed. Following identification procedures, GBRA transfers the benthic macroinvertebrates to 5 mL bottles containing 70-75% Ethyl Alcohol to serve as vouchers for each genus collected.

HZ & MCWE

GBRA provides bottles to HZ and MCWE for bacteriological analyses. HZ and MCWE purchases new bottles for all other samples collected for the Clean Rivers Program. MCWE and HZ maintain electronic copies of certificates from sample container manufacturers for purchased pre-preserved bottles.

- For unpreserved conventional parameters such as TSS and NO₃-NMCWE and HZ use three-liter amber bottles that are purchased new.

- Sample containers for parameters preserved with H₂SO₄ such as TKN, NH₃-N, and Total Phosphorus are one-liter plastic bottles pre-preserved with 2 mL of sulfuric acid that MCWE/ HZ purchases new. MCWE/HZ maintains certificates from sample container manufacturers for purchased bottles electronically.
- GBRA provides 120 mL sterile bottles to HZ/MCWE for bacteriological sampling. HZ collects bacteriological samples in bottles with or without sodium thiosulfate. Samples collected immediately downstream of chlorinated discharges are collected in bottles preserved with sodium thiosulfate.

UGRA

All UGRA sample collection bottles are purchased by UGRA, with exception of 500 mL bottles preserved with sulfuric acid, which are purchased by GBRA and distributed to UGRA. UGRA purchases new and/or cleans and reuses bottles for unpreserved and preserved conventional parameters, with the exception of bottles for TKN, ammonia, and bacteria analysis, which they do not reuse. UGRA staff cleans one-liter unpreserved conventional bottles and one-liter amber bottles for chlorophyll a analysis before sample collection with the following procedure: 1) wash containers with tap water laboratory detergent, 2) triple rinse with hot tap water, and 3) triple rinse with deionized water. UGRA collects bacteriological samples in bottles with sodium thiosulfate. UGRA purchases new bottles for all bacteriological samples and purchases replacement plastic bottles for conventional analysis as needed. Certificates for new bacteriological sample bottles and plastic conventional bottles are maintained in a notebook in the UGRA laboratory. GBRA provides UGRA with new, pre-cleaned, pre-preserved 500 mL bottles for TKN analysis. The GBRA laboratory maintains the manufacturer certificate for these bottles.

- UGRA collects *E. coli* samples in new 120 mL sterile sample bottles. UGRA collects laboratory duplicate samples in 250 mL sterile sample bottles. All *E. coli* sample bottles have been manufacturer certified and pre-preserved with Sodium Thiosulfate.
- Chlorophyll-a and pheophytin samples are collected in 1L brown polyethylene bottles that are either purchased new or are washed and reused using the cleaning procedure described above.
- Unpreserved conventional parameters such as TSS, Turbidity, NO₃-N, Chloride and Sulfate are collected in one-liter plastic bottles that have been purchased new or clean and reused using the cleaning procedure described above.
- UGRA collects TKN samples in new 500 mL plastic bottles that have been manufacturer certified and pre-preserved with one mL of Sulfuric Acid.
- UGRA collects Total Phosphorus samples in 250 mL plastic bottles that are purchased new or washed and reused using the cleaning procedure described above. Prior to use, bottles are acid washed with a solution of equal parts hydrochloric acid and deionized water. Total Phosphorus samples are frozen upon arrival at UGRA laboratory and thawed prior to analysis.
- UGRA collects Ammonia Nitrogen samples in 250 mL plastic bottles that are purchased new. These samples are either analyzed within 24 hours of collection or preserved by the UGRA laboratory with sulfuric acid to a pH of less than 2. If necessary, preservation occurs upon arrival at UGRA laboratory.

Processes to Prevent Contamination

SWQM Procedures outline the necessary steps to prevent contamination of samples, including: direct collection into sample containers, when possible; use of certified containers for organics; and clean sampling techniques for metals. Field QC samples (identified in Section B4) are collected to verify that contamination has not occurred.

Documentation of Field Sampling Activities

Field sampling activities are documented on paper or electronic field data sheets as presented in Appendix D. Data from paper field data sheets are transcribed into the LIMS or an Excel spreadsheet. GBRA transfers data from electronic field data sheets directly into the LIMS via a parsing program or transcribes data from paper field sheets into the LIMS. HZ and MCWE record data electronically or on paper data sheets, which are sent to GBRA. Any paper field sheets are the responsibility of the field technician and are retained by the field technician after the samples are transported and relinquished to the laboratory. GBRA transcribes the HZ and MCWE data into the LIMS. UGRA transcribes field data directly into an Excel spreadsheet. Flow worksheets,

aquatic life use monitoring checklists, habitat assessment forms, field biological assessment forms, and records of bacteriological analyses (if applicable) are part of the field data record. The following will be recorded for all visits:

- Station ID
- Sampling Date
- Location
- Sampling Depth
- Sampling Time
- Sample Collector's name
- Values for all field parameters collected

Additional notes containing detailed observational data not captured by field parameters may include:

- Water appearance
- Weather
- Biological activity
- Recreational activity
- Unusual odors
- Pertinent observations related to water quality or stream uses
- Watershed or instream activities
- Specific sample information
- Missing parameters

Field data is kept in a waterproof field notebook and includes:

- Name of waterbody
- Date and time of sample collection
- Location of sample site (Station ID)
- Time spent electrofishing
- Number of seine hauls

In the biological electronic field sheet (Appendix G) the following are recorded:

- A description of habitats sampled
- Unusual site characteristics
- Field measurements (flow, DO, pH, temperature, specific conductance)

Recording Data

For the purposes of this section and subsequent sections, all field and laboratory personnel follow the basic rules for recording information as documented below:

- Write legibly, in indelible ink.
- Make changes by crossing out original entries with a single line strike-out, entering the changes, and initialing and dating the corrections.
- Close-out incomplete pages with an initialed and dated diagonal line.
- GBRA saves electronic field data sheets as pdf files for posterity.
- GBRA saves electronic laboratory instrumentation calibration and analysis files for posterity.

Sampling Method Requirements or Sampling Process Design Deficiencies, and Corrective Action

Examples of sampling method requirements or sample design deficiencies include but are not limited to such things as inadequate sample volume due to spillage or container leaks, failure to preserve samples appropriately, contamination of a sample bottle during collection, storage temperature and holding time exceedance, sampling at the wrong site, etc. Any deviations from the QAPP, SWQM Procedures, or appropriate sampling procedures may invalidate data and require documented corrective action. Corrective action may include for samples to be

discarded and re-collected. It is the responsibility of the GBRA or UGRA PM, in consultation with the GBRA QAO, UGRA QAO, HZ QAO, or MCWE QAO, to ensure that the actions and resolutions to the problems are documented and that records are maintained in accordance with this QAPP. In addition, these actions and resolutions will be conveyed to the TCEQ CRP PM both verbally and in writing in the project progress reports and by completion of a CAP.

The definition of and process for handling deficiencies and corrective action are defined in Section C1.

Analytical Methods

The analytical methods, associated matrices, and performing laboratories are listed in Appendix A. The authority for analysis methodologies under CRP is derived from the Texas Administrative Code (TAC), Title 30, Chapter 307, in that data generally are generated for comparison to those standards and/or criteria. The TSWQS state “procedures for laboratory analysis must be in accordance with the most recently published edition of the book entitled Standard Methods for the Examination of Water and Wastewater, the TCEQ SWQM Procedures as amended, 40 Code of Federal Regulations (CFR) 136, or other reliable procedures acceptable to the TCEQ, and in accordance with chapter 25 of this title.”

Laboratories collecting data under this QAPP must be accredited by the National Environmental Laboratory Accreditation Program (NELAP) in accordance with TAC, Title 30, Chapter 25. Copies of laboratory quality manuals (QMs) and SOPs shall be made available for review by the TCEQ.

Standards Traceability

All standards used in the field and laboratory are traceable to certified reference materials. Standards preparation is fully documented and maintained in a standards log book. Each documentation includes information concerning the standard identification, starting materials, including concentration, amount used and lot number; date prepared, expiration date and preparer’s initials/signature. The reagent bottle is labeled in a way that will trace the reagent back to preparation.

Analytical Method Deficiencies and Corrective Actions

Deficiencies in field and laboratory measurement systems involve, but are not limited to such things as instrument malfunctions, failures in calibration, blank contamination, quality control samples outside QAPP-defined limits, etc. In many cases, the field technician or lab analyst will be able to correct the problem. If the problem is resolvable by the field technician or lab analyst, then they will document the problem on the field data sheet or laboratory record and complete the analysis. If the problem is not resolvable, then it is conveyed to the applicable Laboratory Director, who will make the determination and notify the applicable laboratory QAO if the problem compromises sample results. If the analytical system failure may compromise the sample results, the resulting data will not be reported to TCEQ. The nature and disposition of the problem is reported on the data report which is sent to the GBRA PM. If a CAP is necessary (Figure C1.1), the GBRA/UGRA QAO will submit the CAP to the TCEQ CRP PM in a timely manner for review. Additionally, the GBRA PM will summarize the CAP in the associated progress report submitted to the TCEQ CRP PM.

The definition of and process for handling deficiencies and corrective action are explained in detail in Section C1.

The TCEQ has determined that analyses associated with qualifier codes (e.g., “holding time exceedance,” “sample received unpreserved,” “estimated value”) may have unacceptable measurement uncertainty associated with them. This will immediately disqualify analyses from submittal to SWQMIS. Therefore, data with these types of problems should not be reported to the TCEQ. Additionally, any data collected or analyzed by means other than those stated in the QAPP, or data suspect for any reason should not be submitted for loading and storage in SWQMIS. However, when data is lost, its absence will be described in the data summary report submitted with the corresponding data set, and a CAP (as described in Section C1) may be necessary.

Acquired Data

Non-directly measured data, secondary data, or acquired data involves the use of data collected under another project and collected with a different intended use than this project. The acquired data still meets the quality requirements of this project and is defined below. The following data source(s) will be used for this project:

Guadalupe-Blanco River Authority FY 26–27 CRP QAPP
Last revised on August 14, 2025

USGS gage station data will be used throughout this project to aid in determining gage height and flow or flow estimate. Rigorous QA checks are completed on gage data by the USGS and the data are approved by USGS and permanently stored at USGS. The LCRA Hydromet gage at Blanco Road is used for flow data for station 12669 and flow estimate data for station 17528. LCRA uses the same procedures as USGS for operation and data quality checks on the Hydromet gages. GBRA calculates the amount of discharge at Dunlap dam, which is used as a flow estimate for stations 12596 and 22189. These data will be submitted to TCEQ under parameter code 00061 (Flow, Instantaneous) or parameter code 74069 (Flow Estimate) depending on the proximity of the monitoring station to the gage stations.

Reservoir stage data are collected every day from the USGS, International Boundary and Water Commission (IBWC), and the United States Army Corps of Engineers (USACE) websites. These data are preliminary and subject to revision. The Texas Water Development Board (TWDB) derives reservoir storage (in acre-feet) from these stage data (elevation in feet above mean sea level), by using the latest rating curve datasets available. These data are published at the TWDB website at <http://waterdatafortexas.org/reservoirs/statewide>. Information about measurement methodology can be found on the TWDB website. These data will be submitted to TCEQ under parameter code 00052 (Reservoir Stage) and parameter code 00053 (Reservoir Percent Full).

B3 Sample Handling and Custody

Sample Tracking

Proper sample handling and custody procedures ensure the custody and integrity of samples beginning at the time of sampling and continuing through transport, sample receipt, preparation, and analysis.

A sample is in custody if it is in actual physical possession or in a secured area that is restricted to authorized personnel. The chain of custody (COC) form is a record that documents the possession of the samples from the time of collection to receipt in the laboratory. The following information concerning the sample is recorded on the COC form (see Appendix E). The following list of items matches the COC form in Appendix E.

- Date and time of collection
- Site identification
- Sample matrix
- Number of containers
- Preservative used
- Was the sample filtered
- Analyses required
- Name of collector
- Custody transfer signatures and dates and time of transfer
- Bill of lading, if applicable

Sample Labeling

Samples from the field are labeled on the container, or on a label, with an indelible marker. Label information includes:

- Site identification
- Date and time of collection
- Preservative added, if applicable
- Sample type (i.e., analyses) to be performed

Sample Handling

Sample Tracking Procedure Deficiencies and Corrective Action

All deficiencies associated with COC procedures, as described in this QAPP, are immediately reported to the GBRA PM. The MCWE/HZ will report any deficiencies to the GBRA PM and QAO and are also subject to GBRA procedures. Deficiencies include such items as delays in transfer resulting in holding time violations; violations

of sample preservation requirements; incomplete documentation, including signatures; possible tampering of samples; broken or spilled samples, etc. The GBRA PM in consultation with the GBRA laboratory QAO will determine if the procedural violation may have compromised the validity of the resulting data. Any failures that have reasonable potential to compromise data validity will invalidate data and the sampling event should be repeated. The resolution of the situation will be reported to the TCEQ CRP PM in the project progress report. CAPs will be prepared by the GBRA/MCWE/HZ QAO, and the GBRA QAO will submit the CAP to the TCEQ CRP PM. UGRA maintains a similar procedure for tracking procedure deficiencies and corrective actions. The UGRA QAO will submit and UGRA CAPS directly to the TCEQ CRP PM.

The definition of and process for handling deficiencies and corrective action are defined in Section C1.

B4 Quality Control

Sampling Quality Control Requirements and Acceptability Criteria

The minimum field QC requirements, and program-specific laboratory QC requirements, are outlined in SWQM Procedures. No field QC samples (field blanks, field duplicates, or trip blanks) will be collected for the Clean Rivers Program.

Laboratory Measurement Quality Control Requirements and Acceptability Criteria

Batch

A batch is defined as environmental samples that are prepared and/or analyzed together with the same process and personnel, using the same lot(s) of reagents. A preparation batch is composed of one to 20 environmental samples of the same NELAP-defined matrix, meeting the above-mentioned criteria and with a maximum time between the start of processing of the first and last sample in the batch to be 24 hours. An analytical batch is composed of prepared environmental samples (extract, digestates, or concentrates) which are analyzed together as a group. An analytical batch can include prepared samples originating from various environmental matrices and can exceed 20 samples.

Method Specific QC requirements

QC samples, other than those specified later in this section (e.g., sample duplicates, surrogates, internal standards, continuing calibration samples, interference check samples, positive control, negative control, and media blank), are run as specified in the methods and in SWQM Procedures. The requirements for these samples, their acceptance criteria or instructions for establishing criteria, and corrective actions are method-specific.

Detailed laboratory QC requirements and corrective action procedures are contained within the individual laboratory QMs. The minimum requirements that all participants abide by are stated below.

Comparison Counting

For routine bacteriological samples, repeat counts on one or more positive samples are required, at least monthly. If possible, the analyst will compare counts with another analyst who also performs the analysis. Replicate counts by the same analyst should agree within 5 percent, and those between analysts should agree within 10 percent. The analyst(s) will record the results.

Limit of Quantitation (LOQ)

The laboratory will analyze a calibration standard (if applicable) at the LOQ published in Appendix A of this QAPP on each day calibrations are performed. In addition, an LOQ check sample will be analyzed with each analytical batch. Calibrations including the standard at the LOQ listed in Appendix A will meet the calibration requirements of the analytical method, or corrective action will be implemented.

LOQ Check Sample

An LOQ check sample consists of a sample matrix (e.g., deionized water, sand, commercially available tissue)

free from the analytes of interest spiked with verified known amounts of analytes or a material containing known and verified amounts of analytes. It is used to establish intra-laboratory bias to assess the performance of the measurement system at the lower limits of analysis. The LOQ check sample is spiked into the sample matrix at a level less than or equal to the LOQ published in Appendix A of this QAPP, for each analyte for each analytical batch of CRP samples run. If it is determined that samples have exceeded the high range of the calibration curve, samples should be diluted or run on another curve. For diluted or high concentration samples run on batches with calibration curves that do not include the LOQ published in Appendix A of this QAPP, a check sample will be run at the low end of the calibration curve.

The LOQ check sample is carried through the complete preparation and analytical process and is performed at a rate of one per analytical batch.

The percent recovery of the LOQ check sample is calculated using the following equation in which %R is percent recovery, S_R is the sample result, and S_A is the reference concentration for the check sample:

$$\%R = S_R / S_A \times 100$$

Measurement performance specifications are used to determine the acceptability of LOQ check sample analyses as specified in Appendix A of this QAPP.

Laboratory Control Sample (LCS)

An LCS consists of a sample matrix (e.g., deionized water, sand, commercially available tissue) free from the analytes of interest spiked with verified known amounts of analytes or a material containing known and verified amounts of analytes. It is used to establish intra-laboratory bias to assess the performance of the measurement system. The LCS is spiked into the sample matrix at a level less than or near the midpoint of the calibration for each analyte. In cases of test methods with very long lists of analytes, LCSs are prepared with all the target analytes and not just a representative number, except in cases of organic analytes with multiplex responses.

The LCS is carried through the complete preparation and analytical process and is performed at a rate of one per preparation batch.

Results of LCSs are calculated by percent recovery (%R), which is defined as 100 times the measured concentration, divided by the true concentration of the spiked sample.

The following formula is used to calculate percent recovery, where %R is percent recovery; S_R is the measured result; and S_A is the true result:

$$\%R = S_R / S_A \times 100$$

Measurement performance specifications are used to determine the acceptability of LCS analyses as specified in Appendix A.

Laboratory Duplicates

A laboratory duplicate is an aliquot taken from the same container as an original sample under laboratory conditions and processed and analyzed independently. A laboratory duplicate is achieved by preparing 2 separate aliquots of a sample, LCS, or matrix spike. Both samples are carried through the entire preparation and analytical process. Laboratory duplicates are used to assess precision and are performed at a rate of one per preparation batch.

For most parameters except bacteria, precision is evaluated using the relative percent difference (RPD) between duplicate results as defined by 100 times the difference (range) of each duplicate set, divided by the average value (mean) of the set. For duplicate results, X_1 and X_2 , the RPD is calculated from the following equation:

$$RPD = \frac{|X_1 - X_2|}{\left(\frac{X_1 + X_2}{2}\right)} \times 100$$

If the precision criterion is exceeded, the data are not acceptable for use under this project and are not reported to TCEQ. Results from all samples associated with that failed duplicate (usually a maximum of 10 samples) are considered to have excessive analytical variability and are qualified as not meeting project QC requirements.

For bacteriological parameters, precision is evaluated using the results from laboratory duplicates. Bacteriological duplicates are analyzed at a 10% frequency (or once per preparation batch, whichever is more frequent). Sufficient volume should be collected to analyze laboratory duplicates from the same sample container.

The base-10 logarithms of the results from the original sample and its duplicate are calculated. The absolute value of the difference between the two base-10 logarithms is calculated and compared to the precision criterion in Appendix A.

$$|\text{Log A} - \text{Log B}| = \text{Log Range}$$

If the difference in logarithms is greater than the precision criterion, the data are not acceptable for use under this project and are not reported to TCEQ. Results from all samples associated with that failed duplicate (usually a maximum of 10 samples) are considered to have excessive analytical variability and are qualified as not meeting project QC requirements.

The precision criterion in Appendix A for bacteriological duplicates applies only to samples with concentrations > 10 MPN.

Matrix spike

Matrix spikes are prepared by adding a known quantity of target analyte to a specified amount of matrix sample for which an independent estimate of target analyte concentration is available.

Matrix spikes indicate the effect of the sample on the precision and accuracy of the results generated using the selected method. Matrix-specific QC samples indicate the effect of the sample matrix on the precision and accuracy of the results generated using the selected method. The information from these controls is sample/matrix specific and would not normally be used to determine the validity of the entire batch. The frequency of matrix spikes is specified by the analytical method, or a minimum of one per preparation batch, whichever is greater. To the extent possible, matrix spikes prepared and analyzed over the course of the project should be performed on samples from different sites.

The components to be spiked shall be as specified by the mandated analytical method. The results from matrix spikes are primarily designed to assess the validity of analytical results in a given matrix and are expressed as percent recovery (%R).

The percent recovery of the matrix spike is calculated using the following equation, where %R is percent recovery, S_{SR} is the concentration measured in the matrix spike, S_R is the concentration in the parent sample, and S_A is the concentration of analyte that was added:

$$\%R = \frac{S_{SR} - S_R}{S_A} \times 100$$

Matrix spike recoveries are compared to the same acceptance criteria established for the associated LCS recoveries, rather than the matrix spike recoveries published in the mandated test method. The EPA 1993 methods (i.e. ammonia-nitrogen, ion chromatography, TKN) that establish matrix spike recovery acceptance criteria are based on recoveries from drinking water that has very low interferences and variability and do not represent the matrices sampled in the CRP. If the matrix spike results are outside laboratory-established criteria, there will be a review of all other associated quality control data in that batch. If all of quality control data in the associated batch passes, it will be the decision of the laboratory QAO or GBRA PM to report the data for the analyte that failed in the parent sample to TCEQ or to determine that the result from the parent sample associated with that failed matrix spike is considered to have excessive analytical variability and does not meet project QC requirements. Depending on the similarities in composition of the samples in the batch, GBRA may consider excluding all of the results in the batch related to the analyte that failed recovery.

Method blank

A method blank is a sample of matrix similar to the batch of associated samples (when available) that is free from the analytes of interest and is processed simultaneously with and under the same conditions as the samples through all steps of the analytical procedures, and in which no target analytes or interferences are present at concentrations that impact the analytical results for sample analyses. The method blank is used to document contamination from the analytical process. The analysis of method blanks should yield values less than the LOQ. For very high-level analyses, the blank value should be less than 5% of the lowest value of the batch, or corrective action will be implemented. Samples associated with a contaminated blank shall be evaluated as to the best corrective action for the samples (e.g., reprocessing, data qualifying codes). In all cases, the corrective action must be documented.

The method blank shall be analyzed at a minimum of one per preparation batch. In those instances for which no separate preparation method is used (e.g., VOA) the batch shall be defined as environmental samples that are analyzed together with the same method and personnel, using the same lots of reagents, not to exceed the analysis of 20 environmental samples.

Quality Control or Acceptability Requirements, Deficiencies, and Corrective Actions

Sampling QC excursions are evaluated by the GBRA or UGRA PM, in consultation with the GBRA or UGRA QAO. In that differences in sample results are used to assess the entire sampling process, including environmental variability, the arbitrary rejection of results based on pre-determined limits is not practical. Therefore, the professional judgment of the GBRA or UGRA PM and QAO will be relied upon in evaluating results.

Laboratory measurement quality control failures are evaluated by the laboratory staff. The disposition of such failures and the nature and disposition of the failure is reported to the Laboratory QAO. The Laboratory QAO will discuss the failure with the GBRA or UGRA QAO. If applicable, the GBRA or UGRA Project Manager or Laboratory QAO will include this information in a CAP and submit the CAP to the TCEQ CRP PM.

The definition of and process for handling deficiencies and corrective action are defined in Section C1.

Additionally, in accordance with CRP requirements and the TNI Standard (Volume 1, Module 2, Section 4.5, Subcontracting of Environmental Tests) when a laboratory that is a signatory of this QAPP finds it necessary and/or advantageous to subcontract analyses, the laboratory that is the signatory on this QAPP must ensure that the subcontracting laboratory is NELAP-accredited (when required) and understands and follows the QA/QC requirements included in this QAPP. This includes confirming that the sub-contracting laboratory has LOQs at or below TCEQ AWRLs and performs all required QC analysis outlined in this QAPP. The signatory laboratory is also responsible for QA of the data prior to delivering it to the GBRA or UGRA, including review of all applicable QC samples related to CRP data. As stated in section 4.5.5 of the TNI Standard, the laboratory performing the subcontracted work shall be indicated in the final report and the signatory laboratory shall make a copy of the subcontractor's report available to the client (GBRA or UGRA) when requested.

B5 Instrument/Equipment Calibration, Testing, Inspection, and Maintenance

All sampling equipment testing and maintenance requirements are detailed in the SWQM Procedures. Sampling equipment is inspected and tested upon receipt and is assured appropriate for use by GBRA field staff and is assured appropriate for use. Equipment records are kept on all field equipment and a supply of critical spare parts is maintained.

All laboratory tools, gauges, instrument, and equipment testing and maintenance requirements are contained within laboratory QM(s).

Instrument Calibration and Frequency

Field equipment calibration requirements are contained in the SWQM Procedures. Post-calibration check error limits and the disposition resulting from errors are adhered to. Data collected from field instruments that do not meet the post-calibration check error limits specified in the SWQM Procedures will not be submitted for inclusion into SWQMIS.

Detailed laboratory calibrations are contained within the QM(s).

B6 Inspection/Acceptance of Supplies and Consumables

No special requirements for acceptance are specified for field sampling supplies and consumables. Reference to the laboratory QM may be appropriate for laboratory-related supplies and consumables.

B7 Data Management

Data Management Process

GBRA field technicians and laboratory personnel follow protocols that ensure that the CRP database maintains its integrity and usefulness. The field technician pre-logs the samples to be collected into the GBRA laboratory information system, which generates separate and distinct sample tracking numbers. Field data collected at the time of the sampling event is logged by the field technician, along with notes on sampling conditions on paper or electronic field data sheets. Any paper field sheets are the responsibility of the field technician and are retained by the field technician after the samples are transported and relinquished to the laboratory. The GBRA lab technician /sample custodian logs the sample in the LIMS database. The separate and distinct sample numbers that the field technician generated for each sample during pre-logging procedures are confirmed upon sample receipt and new numbers are assigned as needed. The sample is always accompanied by a chain of custody. The lab technician /sample custodian must review the chain of custody form to verify that it is filled out correctly and completely. Lab technicians take receipt of the sample and review the chain of custody form, begin sample prep or analysis and transfer samples into the refrigerator for storage. Field data that has been logged on paper field sheets is manually entered into the LIMS by the field technician, once the sample has been successfully received in the LIMS. Field data that has been logged on electronic field sheets are directly exported into the LIMS with a parsing program by the field technician, once the sample has been successfully received in the laboratory information system. An example of the field data sheet and chain of custody form used can be found in Appendices D and E. Twenty-four-hour data recorded by a deployed water quality sensor is downloaded to a personal computer with applicable instrument manufacturer software and transferred to an excel spreadsheet to calculate reported minimum, maximum, and average values. The excel spreadsheet serves as the field data sheet for 24-hour data collections and any data entries into the GBRA LIMS are made from this sheet. Samples that are outsourced to other laboratories are accompanied by a copy of the chain of custody form. The GBRA CRP DM or designee reviews lab bench sheets, outsourced lab data reports and field data sheets for representativeness, quality control, holding times and transcription errors.

Data generated by lab analysts and technicians are logged permanently on analysis bench sheets or generated by instruments in electronic data files. The raw data that is generated by the laboratory analyses are reviewed by the analyst/technician at the bench level, prior to entering or exporting the data into the LIMS. In the review, the analyst/technician verifies that the data includes date and time of analysis, that calculations are correct, that data includes documentation of dilutions and correction factors, that data meets data quality objectives and that the data includes documentation of instrument calibrations, standard curves and control standards. After this review the lab analyst/technician manually inputs or electronically exports the data and quality control information into the LIMS. A second review by another lab analyst/technician of the data entered into the LIMS and supporting documentation validates that the data meets the data quality objectives and that the data includes documentation of instrument calibrations, standard curves and control standards. The GBRA field technician reviews field data prior to entering the data into the GBRA LIMS.

The GBRA Laboratory Director supervises the GBRA laboratory. The Laboratory Director or QAO reviews the report that is generated when all analyses are complete. If the GBRA Lab Director or QAO feel there has been an error or finds that information is missing, the report is returned to the analyst for review and tracking to correct the error and generate a corrected copy. The GBRA DM exports data from the GBRA LIMS, which converts the data to a pipe-delimited text file format acceptable for upload into SWQMIS as described in the latest DMRG. The GBRA DM or designee reviews the respective laboratory and field data for reasonableness after a sample report is completed by the laboratory. If errors or anomalies are found, the GBRA DM notifies the GBRA laboratory QAO and laboratory analyst/technician who created the data, so that the error can be reviewed, tracked and corrected. After the review for reasonableness, the GBRA DM or designee ensures that at least 10% of the data generated by GBRA has been reviewed at the bench level. If at any time the GBRA DM or designee identifies errors, the laboratory data is corrected with and changes are tracked in the GBRA LIMS. The GBRA DM is responsible for transmitting the data to TCEQ in the correct format. The GBRA LIMS creates electronic data deliverable pipe-delimited text files in the event and results file format specified in the DMRG for each sample collected in a given time period and assigns a specific sequenced tag number that pairs the event and results files. The GBRA DM or designee reviews the event and results files, removes non-CRP data, confirms and corrects the submitting entity and collecting entity codes for sub-participants, checks data for correct significant figures and minimum and maximum data outliers. After the data is reviewed for completeness, minimum and maximum data outliers are accepted or rejected after being reviewed and confirmed for validity. The GBRA DM uploads the text files to the SWQMIS test site to screen for data errors. If errors are found by SWQMIS test, the GBRA Data Manager corrects the errors in the events and results files and saves the list of errors as electronic pdf documents. The data files and Data Review Check List are sent to the CRP PM for upload to SWQMIS production environment. If errors are found during the TCEQ review, the GBRA DM corrects those errors and the relevant files are resubmitted to the TCEQ CRP PM.

Samples are taken to SPL or SARA-REL for analyses that cannot be performed by the GBRA laboratory. Data for samples that are outsourced to the SPL or the SARA-REL are received in paper or electronic format, and GBRA staff enters the data into the GBRA LIMS. The data is reviewed by the GBRA Laboratory QAO to confirm that all quality control criteria have been met. After the report has been approved by the GBRA Laboratory QAO, the GBRA DM exports the data from the GBRA LIMS for upload to SWQMIS. The GBRA DM or designee reviews the data for reasonableness and if anomalies are found the SPL or the SARA-REL is contacted to confirm data. If data is confirmed to be correct, then the data exported and transmitted to TCEQ in the same manner as other GBRA laboratory and field data.

UGRA Data Management Process

Field technicians and laboratory personnel follow protocols that ensure that the CRP database maintains its integrity and usefulness. Field data collected at the time of the sampling event is recorded by the field technician, along with notes on sampling conditions on field data sheets. The field data sheet is the responsibility of the field technician and stays in his possession when the samples are transferred to the laboratory. The sample receipt clerk logs the sample in the Lab Samples Database. Each sample is assigned a separate and distinct sample number. The sample is accompanied by a chain of custody form. The sample receipt clerk must review the chain of custody form to verify that it is filled out correctly and completely. Lab analysts take receipt of the sample, begin sample prep or analysis and transfer samples into the refrigerator for storage. The laboratory director reviews the sample information entered into the Lab Samples Database generally within 24 hours of sample receipt. The field data is logged into the CRP database (excel database) by the field technician. Reference to this spreadsheet as the location of the field data is noted in the Lab Sample Database. Examples of the field data sheets and chains of custody used can be found in Appendices D and E. Twenty-four hour data collected by a deployed water quality sonde is downloaded to a personal computer with applicable instrument manufacturer software and transferred to an excel spreadsheet to calculate reported minimum, maximum, and average values. The UGRA field technician transfers the downloaded data to the GBRA field technician by email. The excel spreadsheet serves as the field data sheet for 24-hour data collections and associated data entries into the GBRA LIMS are made from this sheet. Samples that are outsourced to other laboratories are accompanied by a copy of the chain of custody form. The respective DM review the lab bench sheets, outsourced lab data reports and field data sheets for representativeness, quality control, holding times and transcription errors.

Data generated by lab analysts are logged permanently on analysis bench sheets. The data are reviewed by the analyst prior to entering the data into the Lab Samples Database. In the review, the analyst verifies that the data

includes date and time of analysis, that calculations are correct, that data includes documentation of dilutions and correction factors, that data meets data quality objectives and that the data includes documentation of instrument calibrations, standard curves and control standards. After the data is entered by the analyst, the laboratory director validates that the data meets the data quality objectives and that the data includes documentation of instrument calibrations, standard curves and control standards.

Samples are taken to the GBRA lab for analyses that cannot be performed by the UGRA laboratory. Data for samples that are outsourced to the GBRA laboratory are received by UGRA in electronic format. The data is reviewed by the UGRA PM for completeness and the UGRA field technician enters the data into the CRP database (excel database). Reference to this spreadsheet as the location of the outsourced data is noted in the Lab Sample Database. Once all data has been entered into the Lab Sample Database and validated, the report is generated.

The UGRA field technician enters all lab, field, and outsourced data into the CRP database (excel database). The UGRA DM reviews the respective data for reasonableness and if errors or anomalies are found the laboratory or field staff is notified for review and tracking to correct the error. After review for reasonableness, the data is verified to the analysis bench sheets by the UGRA DM. If at any time errors are identified, an amended laboratory report is created with the corrected data and the reason for the amended report is outlined in the case narrative. The Laboratory Samples Database also contains an audit trail function at the individual sample level that records before and after values, date change made, who made the change, and why the change was made. An electronic version of all original and amended reports are retained by the lab. The UGRA DM is responsible for transmitting the data to TCEQ. The UGRA DM creates pipe-delimited text files for the event and results records from the CRP database for each sample and assigns a specific sequenced tag number that pairs the event and results files. After the data is reviewed for completeness, minimum and maximum data outliers are accepted or rejected after being reviewed and confirmed for validity. The UGRA PM uploads the text files to the SWQMIS test site to screen for data errors. If errors are found, the errors are corrected by the UGRA PM. The data files, data checklist, and SWQMIS validator report are sent to the CRP PM in order to be uploaded to SWQMIS. If errors are found after the TCEQ review, those errors are corrected by the UGRA PM.

HZ and MCWE Data Management Process

HZ and MCWE field technicians record the field data on field data sheets electronically or on paper at the time of the sampling event. The samples, along with the chain of custody form, are delivered to the GBRA Laboratory. The GBRA lab technician /sample custodian logs the sample in the GBRA LIMS. Each sample is assigned a separate and distinct sample number. The GBRA lab technician /sample custodian must review the chain of custody form to verify that it is filled out correctly and completely. GBRA lab technicians take receipt of the sample and review the chain of custody form, begin sample prep or analysis and transfer samples into the refrigerator for storage. The HZ and MCWE Field Technician transfers a copy of the calibration/ post-calibration log and field data sheets to the GBRA PM by email. Field data is logged into the GBRA LIMS by the GBRA field technician. Examples of the field data sheets and chains of custody used can be found in Appendices D and E. The GBRA DM or designee reviews the lab bench sheets and field data sheets for HZ and MCWE for representativeness, quality control, holding times and transcription errors. If errors or anomalies are found the HZ or MCWE staff is contacted to investigate the error. Based on the information gathered, the data is invalidated, corrected or validated and if necessary, a corrective action form is initiated.

Data generated by lab analysts and technicians are logged permanently on analysis bench sheets or generated by instruments in electronic data files. The raw data that is generated by the laboratory analyses are reviewed by the analyst/technician at the bench level, prior to entering or exporting the data into the LIMS. In the review, the analyst/technician verifies that the data includes date and time of analysis, that calculations are correct, that data includes documentation of dilutions and correction factors, that data meets data quality objectives and that the data includes documentation of instrument calibrations, standard curves and control standards. After this review the lab analyst/technician manually inputs or electronically exports the data and quality control information into the LIMS. A second review by another lab analyst/technician of the data entered into the LIMS and supporting documentation, validates that the data meets the data quality objectives and that the data includes documentation of instrument calibrations, standard curves and control standards. The GBRA field technician reviews field data prior to entering the data into the GBRA LIMS.

The GBRA Laboratory Director supervises the GBRA laboratory. The Laboratory Director or QAO reviews the report that is generated when all analyses are complete. If the GBRA Lab Director or QAO feel there has been an error or finds that information is missing, the report is returned to the analyst for review and tracking to correct the error and generate a corrected copy. The GBRA DM exports data from the GBRA LIMS, which converts the data to a pipe-delimited text file format acceptable for upload into SWQMIS as described in the latest DMRG. The GBRA DM or designee reviews the respective laboratory and field data for reasonableness after a sample report is completed by the laboratory. If errors or anomalies are found, the GBRA DM notifies the GBRA laboratory QAO and laboratory analyst/technician who created the data, so that the error can be reviewed, tracked and corrected. After the review for reasonableness, the GBRA DM or designee ensures that at least 10% of the data generated by the GBRA has been reviewed at the bench level. If at any time the GBRA DM or designee identifies errors, the laboratory data is corrected with and changes are tracked in the GBRA LIMS. The GBRA DM is responsible for transmitting the HZ and MCWE data to TCEQ in the correct format. The GBRA LIMS creates electronic data deliverable pipe-delimited text files in the event and results file format specified in the DMRG for each sample collected in a given time period and assigns a specific sequenced tag number that pairs the event and results files. The GBRA DM or designee reviews the event and results files, removes non-CRP data, confirms and corrects the submitting entity and collecting entity codes for sub-participants, checks data for correct significant figures and minimum and maximum data outliers. After the data is reviewed for completeness, minimum and maximum data outliers are accepted or rejected after being reviewed and confirmed for validity. The GBRA DM uploads the text files to the SWQMIS test site to screen for data errors. If errors are found by SWQMIS test, the GBRA DM corrects the errors in the events and results files and saves the list of errors as electronic pdf documents. The data files and Data Review Check List are sent to the CRP PM for upload to SWQMIS production environment. If errors are found during the TCEQ review, the GBRA DM corrects those errors and the relevant files are resubmitted to the TCEQ CRP PM.

Data Dictionary

Terminology and field descriptions are included in the 2019 DMRG, or most recent version.

Name of Entity	Tag Prefix	Submitting Entity	Collecting Entity
Guadalupe-Blanco River Authority	GB	GB	GB
Hays County	GB	GB	HZ
Upper Guadalupe River Authority	UG	GB	UG
Meadows Center for Water and the Environment	GB	GB	TI

Data Errors and Loss

The GBRA Laboratory Director supervises the GBRA laboratory and reviews the analytical report that is generated when all analyses are complete. The UGRA Laboratory Director supervises the UGRA lab and reviews the analytical report when all data is complete. The report is reviewed to see that all necessary information is included and that the data quality objectives have been met. When the report is complete, the lab director signs the report. If the lab director or QAO feel there has been an error or finds that information is missing, the report is returned to the analyst for review and tracking to correct the error and generate a corrected copy. The GBRA/UGRA DM reviews the laboratory and field data for reasonableness and if errors or anomalies are found the report is returned to the laboratory director for review and tracking to correct the error. After a review for reasonableness, the data is cross-checked by the GBRA/UGRA DM to ensure that at least 10% of the data generated has been reviewed against project data quality objectives at the bench level. If at any time errors are identified, the LIMS databases are corrected. The GBRA/UGRA DM is responsible for transmitting the data to TCEQ. If errors are found after the TCEQ review, those errors are corrected by the GBRA/UGRA DM. If field or laboratory data are found to fail project QA criteria at any point during the data validation process, then the GBRA/UGRA PM may choose to have the affected data resampled in order to avoid a data loss.

of the files are stored off-site weekly. If the laboratory database or network server fails, the back-up files can be accessed to restore operation or replace corrupted files.

The procedure to minimize data loss for UGRA is similar. All files are stored on the UGRA server and are backed up nightly onsite and to the cloud. If the primary server fails, the back-up files can be accessed to restore operation or replace corrupted files.

Record Keeping and Data Storage

Data is collected and recorded on field data sheets, and transferred into the GBRA LIMS, then the data sheets are filed for review and use later. GBRA uses electronic field sheets, but if there is an error or failure of the tablet and paper field data sheets are used, they are kept for a minimum of one month and then scanned and retained for a minimum of 5 years. Electronic field data sheets are saved as pdf files and retained for a minimum of 5 years. For UGRA, paper field data sheets are used to enter data into the CRP database (excel database) and maintained in paper format for a minimum of 1 month and electronic format for a minimum of 5 years.

The data produced during each analysis is recorded on analysis bench sheets or entered directly into the GBRA LIMS. The information contained in the bench sheets or LIMS electronic file includes all quality control data associated with each day's or batch's analysis. The data on paper logs are transferred to the laboratory database for report generation. If paper bench sheets are used, then they are retained in paper form for a minimum of one month and then scanned for permanent record. For UGRA, the data produced during each analysis is recorded on analysis bench sheets and then entered into the Laboratory Samples Database. The bench sheet includes all quality control data associated with each analysis. The paper bench sheets are retained in paper form for at least one month and electronic format for at least 5 years.

The data reports are generated from data that has been reviewed by the Laboratory QAO or designee and signed by the Laboratory Director. The GBRA/UGRA DM or designee reviews the CRP data generated for verification. If an anomaly or error is found, the DM notifies the Laboratory QAO for review, verification and correction, if necessary. If a correction is made, a tracking log is created in the LIMS. Laboratory reports can be regenerated from the lab database at any time as needed. UGRA maintains permanent pdf files of the lab report.

The LIMS database is housed on the laboratory computer and is backed up on the network server nightly. The GBRA back-up copy of the network server files is made every Friday and that copy is stored off-site at a protected location. All files are stored on the UGRA server and are backed up nightly onsite and to the cloud. The network administrator is responsible for the servers and back up generation.

After data is sent to the TCEQ CRP DM for review, the file that has been created is kept on the network server permanently. The network server is backed up nightly. Paper copies of the data reports are kept for a minimum of one year and then microfilmed for permanent record.

The database containing the scanned images of all lab records is contained on a network server and backed up nightly. A back-up copy of the network server files is made every Friday and that copy for GBRA is stored off-site at a protected location. The GBRA records manager is the custodian of these files. All files are stored on the UGRA server and are backed up nightly onsite and to the cloud.

Data Handling, Hardware, and Software Requirements

The laboratory database is housed on a GBRA server and backed up each evening. The laboratory database uses SQL 2022 database software. The systems are operating in Windows 11 and any additional software needed for word processing, spreadsheet or presentations uses Microsoft 365 Enterprise.

Information Resource Management Requirements

Data will be managed in accordance with the TCEQ DMRG (most recent revision) and applicable Basin Planning Agency information resource management policies.

GPS equipment may be used as a component of the information required by the station location (SLOC) request process for creating the certified positional data that will ultimately be entered into SWQMIS database. Positional data obtained by CRP grantees using a GPS will follow the TCEQ's OPP 8.11 policy regarding the collection and management of positional data. Positional data may be acquired with a GPS and verified with

photo interpolation using a certified source, such as Google Earth or Google Maps. The verified coordinates and map interface can then be used to develop a new SLOC.

C1 Assessments and Response Actions

The following table presents the types of assessments and response actions for data collection activities applicable to the QAPP.

Table C1.1 Assessments and Response Requirements

Assessment Activity	Approximate Schedule	Responsible Party	Scope	Response Requirements
Status Monitoring Oversight, etc.	Continuous	GBRA	Monitoring of the project status and records to ensure requirements are being fulfilled	Report to TCEQ in quarterly report. Submit CAPs to TCEQ as needed.
Monitoring Systems Audit of Basin Planning Agency	Dates to be determined by TCEQ CRP	TCEQ	Field sampling, handling and measurement; facility review; and data management as they relate to CRP	30 days to provide corrective actions response to the TCEQ
Monitoring Systems Audit of Program Subparticipants (UGRA, HZ, & MCWE)	Dates to be determined by GBRA (at least once per biennium)	GBRA	Field sampling, handling and measurement; facility review; and data management as they relate to CRP	30 days to respond in writing to GBRA. GBRA will report findings to TCEQ in progress report.
Laboratory Assessment	Dates to be determined by TCEQ	TCEQ Laboratory Assessor	Analytical and quality control procedures employed at the laboratory and the contract laboratory	30 days to provide corrective actions response to TCEQ

Corrective Action Process for Deficiencies

Deficiencies are any deviation from the QAPP, SWQM Procedures, DMRG, SOPs, or other applicable guidance documents. Deficiencies may invalidate resulting data and require corrective action. Deficiencies that can be prevented from occurring again in the future require a CAP. TCEQ QA staff recognize that deficiencies may occur that are out of the control of GBRA staff and/or their subparticipants' staff. Such deficiencies do not require a CAP. However, when a deficiency impacts data quality or quantity, the TCEQ CRP PM must be notified (within three business days of discovery) and the data loss noted in the associated monitoring activities report and data summary. Corrective action for deficiencies may include for samples to be discarded and re-collected. Deficiencies are documented in logbooks, field data sheets, etc. by field or laboratory staff, are communicated to the GBRA PM (or other appropriate staff) and should be subject to periodic review so their responses can be uniform, and their frequency tracked. It is the responsibility of the GBRA PM, in consultation with the GBRA QAO, to ensure that the actions and resolutions to the problems are documented and that records are maintained in accordance with this QAPP. In addition, these actions and resolutions will be conveyed to the TCEQ CRP PM both verbally and in writing in quarterly progress reports and by completion of a CAP. The GBRA QAO coordinates and maintains CAPs for HZ and MCWE. UGRA maintains a similar corrective actions process for deficiencies.

TCEQ staff are tasked with reviewing CAPs written by GBRA or UGRA concerning deficiencies associated with CRP work. This includes the TCEQ CRP Team Leader, PM, Project QAS, and Lead QAS. The GBRA/UGRA PM or QAO should submit CAPs to their assigned TCEQ CRP PM in a timely manner. GBRA/UGRA can begin implementing corrective actions without TCEQ approval. However, TCEQ may request alternate or modified corrective actions if deemed necessary.

A template for writing CAPs is provided in the [Guidance for Partners in the Texas Clean Rivers Program FY 2026–2027](#) (Exhibit 2C). While CAPs need not adhere to this specific format, they must include information for all of the listed elements. Incomplete CAPs will be returned to the GBRA/UGRA QAO for revision. All CAPs for a FY should be cataloged in the quarterly progress reports submitted to the TCEQ CRP PM by the GBRA/UGRA PM. This documentation should include, at a minimum, the report number, date(s) of deficiency occurrence, description of deficiency, action taken, CAP status, and the date the CAP was closed (if applicable).

Significant conditions that, if uncorrected, could have a serious effect on safety or on the validity or integrity of data will be reported to the TCEQ immediately.

The GBRA/UGRA PM is responsible for ensuring that corrective actions have been implemented and tracks deficiencies and corrective actions. Records of audit findings and corrective actions are maintained by the GBRA/UGRA PM. Audit reports and associated corrective action documentation will be submitted to the TCEQ with the quarterly progress reports.

If audit findings and corrective actions cannot be resolved, then the authority and responsibility for terminating work are specified in the TCEQ QMP and in agreements in contracts between participating organizations.


Corrective Action

CAPs should:

- Identify the problem, nonconformity, or undesirable situation
- Identify immediate remedial actions if possible
- Identify the underlying cause(s) of the problem
- Describe the programmatic impact
- Identify whether the problem is likely to recur, or occur in other areas
- Assist in determining the need for corrective action and actions to prevent reoccurrence
- Employ problem-solving techniques to verify causes, determine solution, and develop an action plan
- Identify personnel responsible for action
- Establish timelines and provide a schedule
- Document the corrective action and action(s) to prevent reoccurrence

A flow chart has been developed to facilitate the process (see Figure C1.1: Corrective Action Process for Deficiencies).

Figure C1.1 Corrective Action Process for Deficiencies

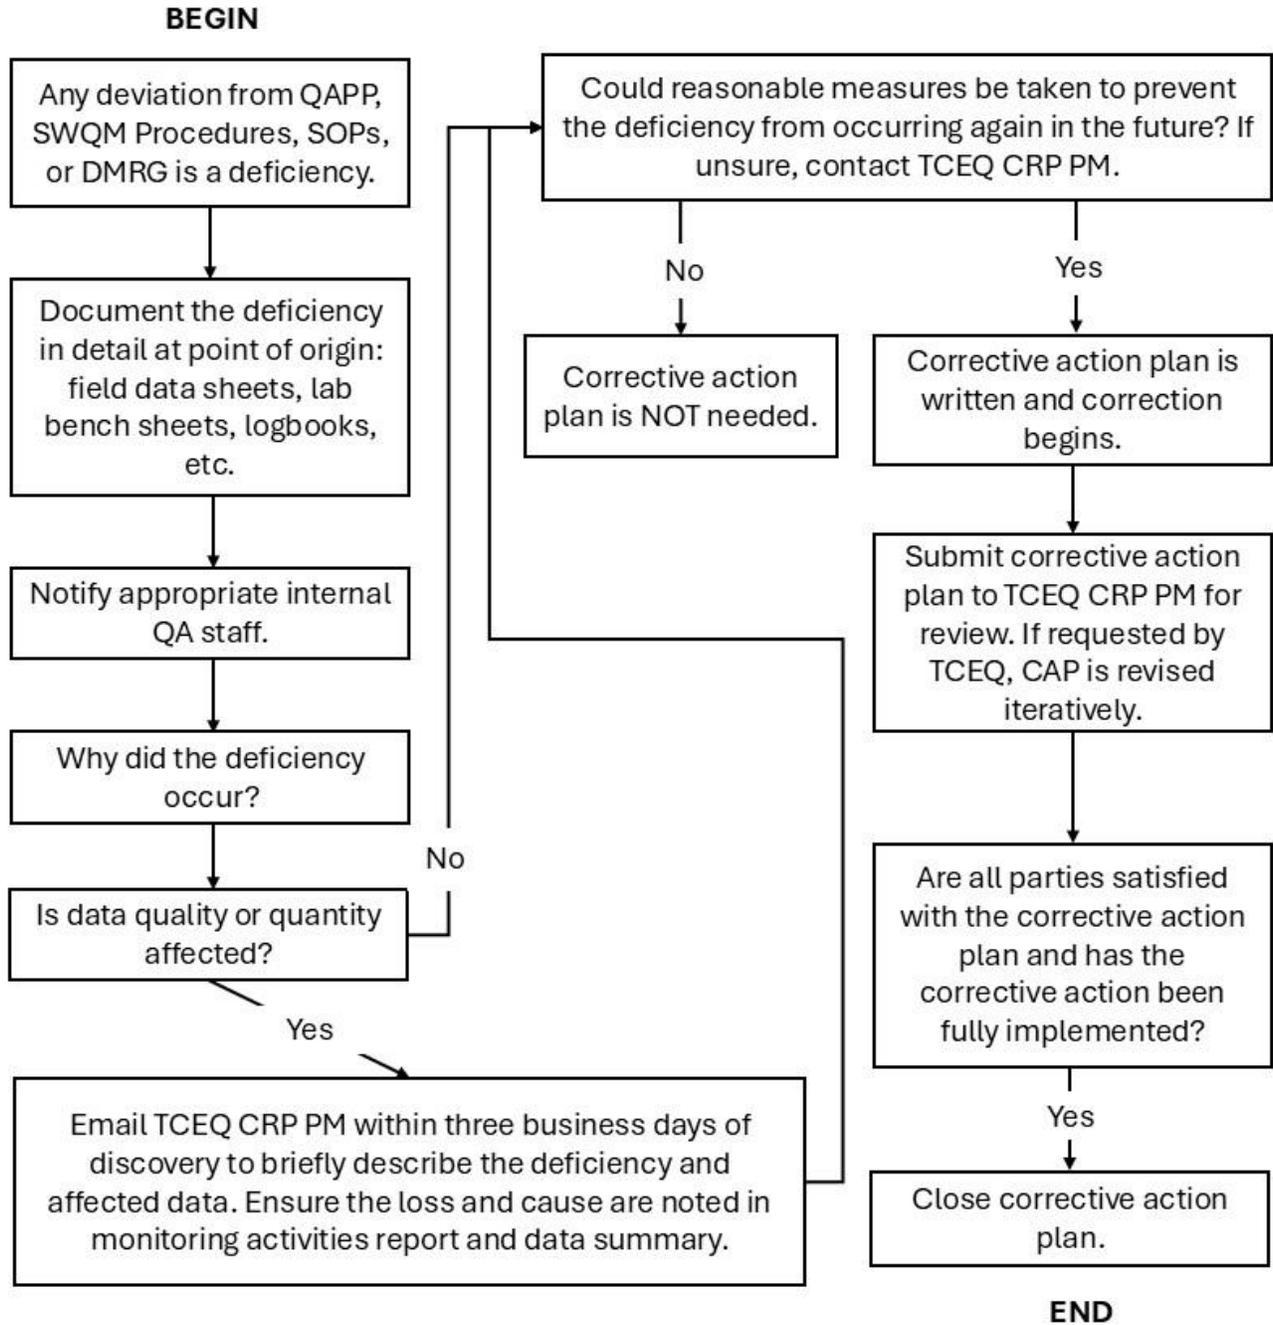

C2 Reports to Management

Table C2.1 QA Management Reports

Type of Report	Frequency (daily, weekly, monthly, quarterly, etc.)	Projected Delivery Date(s)	Person(s) Responsible for Report Preparation	Report Recipients
Non- Conformance Report	As Needed	As Needed	Field Staff Laboratory Staff	GBRA/UGRA QA Staff or Laboratory Management as appropriate
GBRA/UGRA CRP Progress Reports	Quarterly	December 15, 2025 March 15, 2026 June 15, 2026 September 15, 2026 December 15, 2026 March 15, 2027 June 15, 2027 August 15, 2027	GBRA PM	TCEQ CRP PM
Corrective Action Plans (CAPs)	As needed	With Quarterly Report and as Needed	GBRA & UGRA QAOs	GBRA/UGRA PM & TCEQ CRP PM
Data Review Checklist	With Submission of Data to TCEQ	As Needed	GBRA & UGRA DMs	TCEQ CRP PM
HZ/MCWE and UGRA Monitoring Systems Audit Report and Response	As needed, once per biennium for each subparticipant	With Quarterly Report	GBRA QAO	TCEQ CRP PM
HZ Monitoring Systems Audit Response	After Audit Report Received by HZ	Within 30 days of receiving Audit Report.	HZ QAO	GBRA PM
MCWE Monitoring Systems Audit Response	After Audit Report Received by MCWE	Within 30 days of receiving Audit Report.	MCWE QAO	GBRA PM
UGRA Monitoring Systems Audit Response	After Audit Report Received by UGRA	Within 30 days of receiving Audit Report. t	UGRA CRP PM	GBRA PM
Data Summary	With Submission of Data to TCEQ	As Needed	GBRA/UGRA DM	TCEQ CRP PM

Reports to GBRA Project Management

The GBRA Laboratory QAO will report any sample or data issue to the GBRA PM. The GBRA Field Technician will report any sample or data issue associated with the field data to the GBRA PM. The HZ or MCWE field technician will report any data issues to the GBRA PM. The UGRA PM submits quarterly

reports of progress with known data issues and requests for expense reimbursements to the GBRA PM. Issues can include but are not limited to, loss of data, data anomalies or outliers, equipment failures or delays in meeting holding times. Based on the discussions, appropriate action will be taken (report data as is, resample, qualify the data, or report a loss of data). A corrective action report will be generated if any action is taken due to a failure in the quality system.

Reports to TCEQ Project Management

All reports detailed in this section are contract deliverables and are transferred to the TCEQ in accordance with contract requirements.

Progress Report

Summarizes the GBRA/UGRA's activities for each task; reports monitoring status, problems, delays, deficiencies, status of open CAPs, and documentation for completed CAPs; and outlines the status of each task's deliverables.

Monitoring Systems Audit Report and Response

Following any audit performed by the GBRA, a report of findings, recommendations and response is sent to the TCEQ in the quarterly progress report.

Data Summary

Contains basic identifying information about the data set and comments regarding inconsistencies and errors identified during data verification and validation steps or problems with data collection efforts (e.g., deficiencies).

Reports by TCEQ Project Management

Contractor Evaluation

The GBRA participates in a contractor evaluation by the TCEQ annually for compliance with administrative and programmatic standards. Results of the evaluation are submitted to the TCEQ Financial Administration Division, Procurement and Contracts Section.

D1 Data Review, Verification, and Validation

All field and laboratory data will be reviewed and verified for integrity, continuity, reasonableness, and conformance to project requirements, and then validated against the project objectives and measurement performance specifications which are listed in Section A6 of this QAPP. Only those data which are supported by appropriate quality control data and meet the measurement performance specifications defined for this project will be considered acceptable and will be reported to the TCEQ for entry into SWQMIS.

Verification and Validation Methods

All field and laboratory data will be reviewed, verified and validated to ensure they conform to project specifications.

Data review, verification, and validation will be performed using self-assessments as well as peer and management review as appropriate to the project task. The data review tasks to be performed by field and laboratory staff are listed in the first two columns of Table D1.1-D.4 respectively. Potential errors are identified by examination of documentation and by manual examination of corollary or unreasonable data; this analysis may be computer-assisted. If a question arises or an error is identified, the manager of the task responsible for generating the data is contacted to resolve the issue. Issues which can be corrected are corrected and documented. If an issue cannot be corrected, the task manager consults with the higher-level project management to establish the appropriate course of action, or the data associated with the issue are rejected and not reported to the TCEQ for storage in SWQMIS. Field and laboratory reviews, verifications, and validations are documented.

After the field and laboratory data are reviewed, another level of review is performed once the data are combined into a data set. This review step, as specified in Tables D1.1-D1.4, is performed by the GBRA or UGRA DM. Data review, verification, and validation tasks to be performed on the data set include, but are not limited to, the confirmation of laboratory and field data review, evaluation of field QC results, additional evaluation of anomalies and outliers, analysis of sampling and analytical gaps, and confirmation that all parameters and sampling sites are included in the QAPP.

The Data Review Checklist (see Appendix F) covers three main types of review: data format and structure, data quality review, and documentation review. The Data Review Checklist is completed and sent with the water quality data submitted to the TCEQ to ensure that the review process is being performed.

Another element of the data validation process is consideration of any findings identified during the monitoring systems audit conducted by the TCEQ CRP Lead QAS. Any issues requiring corrective action must be addressed, and the potential impact of these issues on previously collected data will be assessed. After the data are reviewed and documented, the GBRA/UGRA PM validates that the data meet the data quality objectives of the project and are suitable for reporting to TCEQ.

If any requirements or specifications of the CRP are not met, based on any part of the data review, the responsible party should document the nonconforming activities and submit the information to the GBRA/UGRA DM with the data in the data summary (See Appendix F). All failed QC checks, missing samples, missing analytes, missing parameters, and suspect results should be discussed in the data summary.

Table D1.1: GBRA Data Review Tasks

Data to be Verified	Field Task	Laboratory Task	QA Task	Lead Organization Data Manager Task
Sample documentation complete; samples labeled, sites identified	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ QAO	GBRA DM
Standards and reagents traceable	GBRA Field Technician	GBRA Laboratory Director/ Lab QAO	GBRA PM/ QAO	
Chain of custody complete/acceptable	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ QAO	
NELAP Accreditation is current		GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	
Sample preservation and handling acceptable	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	
Holding times not exceeded	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	
Collection, preparation, and analysis consistent with SOPs and QAPP	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
Field documentation (e.g., biological, stream habitat) complete	GBRA Field Technician		GBRA PM/Q AO	GBRA DM
Instrument calibration data complete	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
QC samples analyzed at required frequency	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/QAO	GBRA DM
QC results meet performance and program specifications	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/Q AO/Lab Director / Lab QAO	GBRA DM
Analytical sensitivity (LOQ/AWRL) consistent with QAPP	GBRA Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/QAO/ Lab Director/ Lab QAO	GBRA DM
Results, calculations, transcriptions	GBRA Field Technician	GBRA Laboratory	GBRA Lab Director /	GBRA DM

checked		Analyst/ Technician	Lab QAO	
Laboratory bench-level review performed		GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
All laboratory samples analyzed for all scheduled parameters		GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
Corollary data agree			GBRA PM/ QAO	GBRA DM
Nonconforming activities documented	GBRA Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Outliers confirmed and documented; reasonableness check performed	GBRA Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Dates formatted correctly	GBRA Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Depth reported correctly and in correct units	GBRA Field Technician		GBRA Lab Director / Lab QAO	GBRA DM
TAG IDs correct				GBRA DM
TCEQ Station ID number assigned				GBRA DM
Valid parameter codes				GBRA DM
Codes for submitting entity(ies), collecting entity(ies), and monitoring type(s) used correctly				GBRA DM
Time based on 24-hour clock	GBRA Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Check for transcription errors	GBRA Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Sampling and analytical data gaps checked (e.g., all sites for which data are reported are on the coordinated monitoring schedule)	GBRA Field Technician			GBRA DM
Field instrument pre- and post-calibration check results within limits	GBRA Field Technician		GBRA PM/QAO	GBRA DM
10% of data manually reviewed				GBRA DM

Table D1.2: UGRA Data Review Tasks

Data to be Verified	Field Task	Laboratory Task	QA Task	Lead Organization Data Manager Task
Sample documentation complete; samples labeled, sites identified	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA PM/ QAO	UGRA DM
Standards and reagents traceable	UGRA Field Technician	UGRA Laboratory Director/ Lab QAO	UGRA PM/ QAO	
Chain of custody complete/acceptable	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA PM/ QAO	
NELAP Accreditation is current		UGRA Laboratory Analyst/ Technician	UGRA Lab Manager/ QAO	
Sample preservation and handling acceptable	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA Director / QAO	
Holding times not exceeded	UGRA Field Technician	GBRA Laboratory Analyst/ Technician	UGRA Lab Director/ QAO	
Collection, preparation, and analysis consistent with SOPs and QAPP	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA Lab Director/ QAO	UGRA DM
Field documentation (e.g., biological, stream habitat) complete	UGRA Field Technician		UGRA PM/ QAO	UGRA DM
Instrument calibration data complete	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA Lab Director / QAO	UGRA DM
QC samples analyzed at required frequency	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA PM/ QAO	UGRA DM
QC results meet performance and program specifications	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	UGRA PM/ QAO/Lab Director / Lab QAO	UGRA DM
Analytical sensitivity (LOQ/AWRL) consistent with QAPP	UGRA Field Technician	UGRA Laboratory Analyst/ Technician	GBRA PM/ QAO/Lab Director / QAO	UGRA DM
Results, calculations,	UGRA Field	UGRA Laboratory	UGRA Lab	UGRA DM

transcriptions checked	Technician	Analyst/ Technician	Director/ QAO	
Laboratory bench-level review performed		UGRA Laboratory Analyst/ Technician	UGRA Lab Director/ QAO	UGRA DM
All laboratory samples analyzed for all scheduled parameters		UGRA Laboratory Analyst/ Technician	UGRA Lab Director/ QAO	UGRA DM
Corollary data agree			UGRA PM/ QAO	UGRA DM
Nonconforming activities documented	UGRA Field Technician	UGRA Laboratory Analyst/ Technician		UGRA DM
Outliers confirmed and documented; reasonableness check performed	UGRA Field Technician	UGRA Laboratory Analyst/ Technician		UGRA DM
Dates formatted correctly	UGRA Field Technician	UGRA Laboratory Analyst/ Technician		UGRA DM
Depth reported correctly and in correct units	UGRA Field Technician		UGRA Lab Director/ QAO	UGRA DM
TAG IDs correct				UGRA DM
TCEQ Station ID number assigned				UGRA DM
Valid parameter codes				UGRA DM
Codes for submitting entity(ies), collecting entity(ies), and monitoring type(s) used correctly				UGRA DM
Time based on 24-hour clock	UGRA Field Technician	UGRA Laboratory Analyst/ Technician		UGRA DM
Check for transcription errors	UGRA Field Technician	UGRA Laboratory Analyst/ Technician		UGRA DM
Sampling and analytical data gaps checked (e.g., all sites for which data are reported are on the coordinated monitoring schedule)	UGRA Field Technician			UGRA DM
Field instrument pre- and post-calibration check results within limits	UGRA Field Technician		UGRA PM/ QAO	UGRA DM
10% of data manually reviewed				UGRA DM

Table D1.3: HZ Data Review Tasks

Data to be Verified	Field Task	Laboratory Task	QA Task	Lead Organization Data Manager Task
Sample documentation complete; samples labeled, sites identified	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ HZ QAO	GBRA DM
Standards and reagents traceable	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ HZ QAO	
Chain of custody complete/acceptable	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director /Lab QAO	
NELAP Accreditation is current		GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	
Sample preservation and handling acceptable	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director/ Lab QAO	
Holding times not exceeded	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director/ Lab QAO	
Collection, preparation, and analysis consistent with SOPs and QAPP	HZ Field Technician	GBRA Laboratory Analyst/Tec hnician	GBRA Lab Director/ Lab QAO	GBRA DM
Field documentation (e.g., biological, stream habitat) complete	HZ Field Technician		GBRA PM/ HZ QAO	GBRA DM
Instrument calibration data complete	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
QC samples analyzed at required frequency	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ HZ QAO	GBRA DM
QC results meet performance and program specifications	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ HZ QAO/Lab Director/ Lab QAO	GBRA DM
Analytical sensitivity (LOQ/AWRL) consistent with QAPP	HZ Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ HZ QAO/Lab Director / QAO	GBRA DM
Results, calculations, transcriptions	HZ Field	GBRA Laboratory	GBRA Lab Director	GBRA DM

checked	Technician	Analyst/ Technician	/Lab QAO	
Laboratory bench-level review performed		GBRA Laboratory Analyst/ Technician	GBRA Lab Director /Lab QAO	GBRA DM
All laboratory samples analyzed for all scheduled parameters		GBRA Laboratory Analyst/ Technician	GBRA Lab Director /Lab QAO	GBRA DM
Corollary data agree			GBRA PM/ HZ QAO	GBRA DM
Nonconforming activities documented	HZ Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Outliers confirmed and documented; reasonableness check performed	HZ Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Dates formatted correctly	HZ Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Depth reported correctly and in correct units	HZ Field Technician		GBRA Lab Director/Lab QAO	GBRA DM
TAG IDs correct				GBRA DM
TCEQ Station ID number assigned				GBRA DM
Valid parameter codes				GBRA DM
Codes for submitting entity(ies), collecting entity(ies), and monitoring type(s) used correctly				GBRA DM
Time based on 24-hour clock	HZ Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Check for transcription errors	HZ Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Sampling and analytical data gaps checked (e.g., all sites for which data are reported are on the coordinated monitoring schedule)	HZ Field Technician			GBRA DM
Field instrument pre- and post-calibration check results within limits	HZ Field Technician		GBRA PM/ HZ QAO	GBRA DM
10% of data manually reviewed				GBRA DM

Table D1.4: MCWE Data Review Tasks

Data to be Verified	Field Task	Laboratory Task	QA Task	Lead Organization Data Manager Task
Sample documentation complete; samples labeled, sites identified	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ MCWE QAO	GBRA DM
Standards and reagents traceable	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ MCWE QAO	
Chain of custody complete/acceptable	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director/ Lab QAO	
NELAP Accreditation is current		GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	
Sample preservation and handling acceptable	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	
Holding times not exceeded	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	UGRA Lab Director/ Lab QAO	
Collection, preparation, and analysis consistent with SOPs and QAPP	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
Field documentation (e.g., biological, stream habitat) complete	MCWE Field Technician		GBRA PM/ MCWE QAO	GBRA DM
Instrument calibration data complete	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
QC samples analyzed at required frequency	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ MCWE QAO	GBRA DM
QC results meet performance and program specifications	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ MCWE QAO/Lab Director / Lab QAO	GBRA DM
Analytical sensitivity (LOQ/AWRL) consistent with QAPP	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA PM/ MCWE QAO/Lab Director / QAO	GBRA DM

Results, calculations, transcriptions checked	MCWE Field Technician	GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
Laboratory bench-level review performed		GBRA Laboratory Analyst/ Technician	GBRA Lab Director / Lab QAO	GBRA DM
All laboratory samples analyzed for all scheduled parameters		GBRA Laboratory Analyst/ Technician	GBRA Lab Director/ Lab QAO	GBRA DM
Corollary data agree			GBRA PM/ MCWE QAO	GBRA DM
Nonconforming activities documented	MCWE Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Outliers confirmed and documented; reasonableness check performed	MCWE Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Dates formatted correctly	MCWE Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Depth reported correctly and in correct units	MCWE Field Technician		GBRA Lab Director / Lab QAO	GBRA DM
TAG IDs correct				GBRA DM
TCEQ Station ID number assigned				GBRA DM
Valid parameter codes				GBRA DM
Codes for submitting entity(ies), collecting entity(ies), and monitoring type(s) used correctly				GBRA DM
Time based on 24-hour clock	MCWE Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Check for transcription errors	MCWE Field Technician	GBRA Laboratory Analyst/ Technician		GBRA DM
Sampling and analytical data gaps checked (e.g., all sites for which data are reported are on the coordinated monitoring schedule)	MCWE Field Technician			GBRA DM
Field instrument pre- and post-calibration check results within limits	MCWE Field Technician		GBRA PM/ MCWE QAO	GBRA DM
10% of data manually reviewed				GBRA DM

D2 Reconciliation with User Requirements

Data produced in this project, and data collected by other organizations (e.g., USGS, TCEQ, etc.), will be analyzed and reconciled with project data quality requirements. Data which do not meet requirements will not be submitted to SWQMIS nor will be considered appropriate for any of the uses noted in Section A4.

Appendix A: Measurement Performance Specifications (Table A6.1a–4d)

Measurement performance specifications define the data quality needed to satisfy project objectives. To this end, measurement performance specifications are qualitative and quantitative statements that:

- clarify the intended use of the data
- define the type of data needed to support the end use
- identify the conditions under which the data should be collected

Appendix A of the QAPP addresses measurement performance specifications, including:

- analytical methodologies
- AWRLs
- limits of quantitation
- bias limits for LCSs
- precision limits for laboratory control sample duplicates (LCSDs)
- completeness goals
- qualitative statements regarding representativeness and comparability

The items identified above should be considered for each type of monitoring activity. The CRP encourages that data be collected to address multiple objectives to optimize resources; however, caution should be applied when attempting to collect data for multiple purposes because measurement performance specifications may vary according to the purpose. For example, limits of quantitation may differ for data used to assess standards attainment and for trend analysis. When planning projects, first priority will be given to the main use of the project data and the data quality needed to support that use, then secondary goals will be considered.

Table A6.1-4 reflects actual parameters, methods, etc. employed by the GBRA and its participants. Procedures for laboratory analysis must be in accordance with the most recently published edition of Standard Methods for the Examination of Water and Wastewater, 40 CFR 136, or otherwise approved independently. Only data collected that have a valid TCEQ parameter code assigned in Tables A6 are stored in SWQMIS. Any parameters listed in Tables A6 that do not have a valid TCEQ parameter code assigned will not be stored in SWQMIS.

Table A6.1–4 : Measurement Performance Specifications

TABLE A6.1a Measurement Performance Specifications for GBRA

Field Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
TEMPERATURE, WATER (DEGREES CENTIGRADE)	DEG C	water	SM 2550 B and TCEQ SOP V1	00010	GBRA Field
TRANSPARENCY, SECCHI DISC (METERS)****	meters	water	TCEQ SOP V1	00078	GBRA Field
SPECIFIC CONDUCTANCE, FIELD (US/CM @ 25C)	us/cm	water	EPA 120.1 and TCEQ SOP, V1	00094	GBRA Field
OXYGEN, DISSOLVED (MG/L)	mg/L	water	SM 4500-O G and TCEQ SOP V1	00300	GBRA Field
PH (STANDARD UNITS)	s.u.	water	EPA 150.1 and TCEQ SOP V1	00400	GBRA Field
SALINITY - PARTS PER THOUSAND***	PPT	water	SM 2520 and TCEQ SOP V1	00480	GBRA Field
DAYS SINCE PRECIPITATION EVENT (DAYS)	days	other	TCEQ SOP V1	72053	GBRA Field
DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE*	meters	water	TCEQ SOP V2	82903	GBRA Field
RESERVOIR STAGE (FEET ABOVE MEAN SEA LEVEL)**	FT ABOVE MSL	water	TWDB	00052	GBRA Field
RESERVOIR PERCENT FULL**	% RESERVOIR CAPACITY	water	TWDB	00053	GBRA Field
RESERVOIR ACCESS NOT POSSIBLE LEVEL TOO LOW ENTER 1 IF REPORTING	NS	other	TCEQ Drought Guidance	00051	GBRA Field
MAXIMUM POOL WIDTH AT TIME OF STUDY (METERS)*	meters	other	TCEQ SOP V2	89864	GBRA Field
MAXIMUM POOL DEPTH AT TIME OF STUDY(METERS)*	meters	other	TCEQ SOP V2	89865	GBRA Field
POOL LENGTH, METERS*	meters	other	TCEQ SOP V2	89869	GBRA Field
% POOL COVERAGE IN 500 METER REACH*	%	other	TCEQ SOP V2	89870	GBRA Field

* To be routinely reported when collecting data from perennial pools.
 ** As published by the Texas Water Development Board on their website
<https://www.waterdatafortexas.org/reservoirs/statewide>
 ***Salinity only collected at tidally influenced stations
 **** Transparency only collected at reservoir stations

References:

United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).
 TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).

TABLE A6.1b Measurement Performance Specifications for GBRA					
Flow Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
FLOW STREAM, INSTANTANEOUS (CUBIC FEET PER SEC)	cfs	water	TCEQ SOP V1	00061	GBRA Field
FLOW SEVERITY: 1=No Flow,2=Low,3=Normal,4=Flood,5=High,6=Dry	NU	water	TCEQ SOP V1	01351	GBRA Field
STREAM FLOW ESTIMATE (CFS)*	cfs	Water	TCEQ SOP V1	74069	GBRA Field
FLOW MTH 1=GAGE 2=ELEC 3=MECH 4=WEIR/FLU 5=DOPPLER	NU	other	TCEQ SOP V1	89835	GBRA Field
<p>*In cases where a direct flow measurement may not be possible and there are no USGS flow gages representative of conditions at the monitoring site, discharge data from the nearest flow gage is submitted as a flow estimate. See Table B1.1.</p> <p>References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).</p>					

TABLE A6.1c Measurement Performance Specifications for GBRA
Conventional Parameters in Water

Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Precision (RPD)	Bias %Rec. of LCS	Lab
RESIDUE, TOTAL NONFILTRABLE (MG/L)	mg/L	water	SM 2540D	00530	5	1**	NA	NA	NA	GBRA, SPL, SARA-REL***
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	EPA 350.1 Rev. 2.0 (1993)	00610	0.1	0.1	70-130	20	80-120	GBRA and SPL***
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	SM4500 NH3D	00610	0.1	0.1	70-130	20	80-120	SARA-REL***
NITRATE NITROGEN, TOTAL (MG/L AS N)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00620	0.05	0.05	70-130	20	80-120	GBRA, SPL, SARA-REL***
NITRITE NITROGEN, TOTAL (MG/L AS N)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00615	0.05	0.05	70-130	20	80-120	GBRA, SPL, SARA-REL***
NITROGEN, KJELDAHL, TOTAL (MG/L AS N)	mg/L	water	EPA 351.2 Rev. 2 (1993)	00625	0.2	0.2	70-130	20	80-120	GBRA, SPL, SARA-REL***
PHOSPHORUS, TOTAL, WET METHOD (MG/L AS P)	mg/L	water	EPA 365.3	00665	0.06	0.02	70-130	20	80-120	GBRA and SPL, SARA-REL***
HARDNESS, TOTAL (MG/L AS CaCO3)*	mg/L	water	SM 2340 C	00900	5	5	NA	20	80-120	GBRA, SPL, SARA-REL***
CHLORIDE (MG/L AS CL)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00940	5	1	70-130	20	80-120	GBRA and SPL***
CHLORIDE (MG/L AS CL)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00940	5	5	70-130	20	80-120	SARA-REL***
SULFATE (MG/L AS SO4)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00945	5	1	70-130	20	80-120	GBRA and SPL***
SULFATE (MG/L AS SO4)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00945	5	5	70-130	20	80-120	SARA-REL***
CHLOROPHYLL-A UG/L SPECTROPHOTOMETRIC ACID. METH	ug/L	water	SM 10200-H4	32211	3	1	NA	20	80-120	GBRA***
CHLOROPHYLL-A UG/L SPECTROPHOTOMETRIC ACID. METH	ug/L	water	SM 10200-H	32211	3	1	NA	20	80-120	SARA-REL***

CHLOROPHYLL-A, FLUOROMETRIC METHOD, UG/L	µg/L	water	EPA 445.0	70953	3	1	NA	20	80- 120	SPL ***
PHEOPHYTIN-A UG/L SPECTROPHOTOMETRIC ACID. METH.	µg/L	water	SM 10200- H4	32218	3	1	NA	NA	NA	GBRA ***
PHEOPHYTIN-A UG/L SPECTROPHOTOMETRIC ACID. METH.	µg/L	water	SM 10200-H	32218	3	1	NA	NA	NA	SARA-REL ***
PHEOPHYTIN-A UG/L FLUOROMETRIC METHOD	µg/L	water	EPA 445	32213	3	1	NA	NA	NA	SPL ***
TURBIDITY,LAB NEPHELOMETRIC TURBIDITY UNITS, NTU	NTU	water	SM 2130B	82079	0.5	0.5	NA	NA	NA	GBRA and SPL ***
TURBIDITY,LAB NEPHELOMETRIC TURBIDITY UNITS, NTU	NTU	water	EPA 180.1	82079	0.5	0.5	NA	NA	NA	SARA-REL ***
<p>*Hardness is not used for regulatory purposes but is used to assess metals in water at inland sites (estuarine sites do not require hardness analysis). **TSS LOQ is based on the volume of sample used. ***SPL or SARA-REL laboratories will be used in the event of an equipment failure and the need to meet holding times.</p> <p>References:United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).</p>										

TABLE A6.1d Measurement Performance Specifications for GBRA

Bacteriological Parameters in Water

Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Log Difference of Duplicates	Bias %Rec. of LCS	Lab
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	IDEXX Laboratories Colilert®- 18**	31699	1	1	NA	0.50*	NA	GBRA* **
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	SM 9223-B IDEXX**	31699	1	1	NA	0.50*	NA	SPL and SARA- REL***
E.COLI, COLILERT, IDEXX, HOLDING TIME	hours	water	NA	31704	NA	NA	NA	NA	NA	GBRA, SPL, SARA- REL***

* This value is not expressed as a relative percent difference. It represents the maximum allowable difference between the logarithm of the result of a sample and the logarithm of the duplicate result. See Section B4.
 ** *E. coli* samples analyzed by these methods should always be processed as soon as possible and within 8 hours. When transport conditions necessitate delays in delivery longer than 6 hours, the holding time may be extended and samples must be processed as soon as possible and within 30 hours.
 ***SPL or SARA-REL laboratories will be used in the event of an equipment failure and the need to meet holding times.

References:

Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version
 Annual Book of ASTM Standards, Section 11, Water and Environmental Technology, Volume 11.02, Water
 TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).

TABLE A6.1e Measurement Performance Specifications for GBRA

24 Hour Parameters in Water					
Parameter	Units	Matrix	Method	Parameter Code	Lab
TEMPERATURE, WATER (DEGREES CENTIGRADE), 24HR AVG	DEG C	Water	TCEQ SOP V1	00209	GBRA field
WATER TEMPERATURE, DEGREES CENTIGRADE, 24HR MAX	DEG C	Water	TCEQ SOP V1	00210	GBRA field
TEMPERATURE, WATER (DEGREES CENTIGRADE) 24HR MIN	DEG C	Water	TCEQ SOP V1	00211	GBRA field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR AVG	uS/cm	Water	TCEQ SOP V1	00212	GBRA field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR MAX	uS/cm	Water	TCEQ SOP V1	00213	GBRA field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR MIN	uS/cm	Water	TCEQ SOP V1	00214	GBRA field
PH, S.U., 24HR MAXIMUM VALUE	std. units	Water	TCEQ SOP V1	00215	GBRA field
PH, S.U., 24HR, MINIMUM VALUE	std. units	Water	TCEQ SOP V1	00216	GBRA field
SALINITY, 24-HR, MAXIMUM, PPT	ppt	Water	TCEQ SOP V1	00217	GBRA field
SALINITY, 24-HR, AVERAGE, PPT	ppt	Water	TCEQ SOP V1	00218	GBRA field
SALINITY, 24-HR, MINIMUM, PPT	ppt	Water	TCEQ SOP V1	00219	GBRA field
SALINITY, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00220	GBRA field
WATER TEMPERATURE, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00221	GBRA field

SPECIFIC CONDUCTANCE, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00222	GBRA field
pH, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00223	GBRA field
DISSOLVED OXYGEN, 24-HOUR MIN. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89855	GBRA field
DISSOLVED OXYGEN, 24-HOUR MAX. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89856	GBRA field
DISSOLVED OXYGEN, 24-HOUR AVG. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89857	GBRA field
DISSOLVED OXYGEN, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	89858	GBRA field
References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).					

TABLE A6.1f Measurement Performance Specifications for GBRA						
Biological - Habitat						
Parameter	Units	Matrix	Method	Parameter Code	Lab	
FLOW STREAM, INSTANTANEOUS (CUBIC FEET PER SEC)	cfs	Water	TCEQ SOP V2	00061	GBRA	
BIOLOGICAL DATA	NS	Other	NA/Calculation	89888	GBRA	
STREAM TYPE; 1=PERENNIAL 2=INTERMITTENT S/PERENNIAL POOLS 3=INTERMITTENT 4=UNKNOWN	NU	Water	NA/Calculation	89821	GBRA	
STREAMBED SLOPE (M/KM)	M/KM	Other	NA/Calculation	72051	GBRA	
AVERAGE PERCENTAGE INSTREAM COVER	%	Other	TCEQ SOP V2	84159	GBRA	
STREAM ORDER	NU	Water	TCEQ SOP V2	84161	GBRA	
NUMBER OF LATERAL TRANSECTS MADE	NU	Other	TCEQ SOP V2	89832	GBRA	
FLOW MTH 1=GAGE 2=ELEC 3=MECH 4=WEIR/FLU 5=DOPPLER	NU	Other	TCEQ SOP V2	89835	GBRA	
TOTAL NUMBER OF STREAM BENDS	NU	Other	TCEQ SOP V2	89839	GBRA	

NUMBER OF WELL DEFINED STREAM BENDS	NU	Other	TCEQ SOP V2	89840	GBRA
NUMBER OF MODERATELY DEFINED STREAM BENDS	NU	Other	TCEQ SOP V2	89841	GBRA
NUMBER OF POORLY DEFINED STREAM BENDS	NU	Other	TCEQ SOP V2	89842	GBRA
TOTAL NUMBER OF RIFFLES	NU	Other	TCEQ SOP V2	89843	GBRA
DOMINANT SUBSTRATE TYPE(1=CLAY,2=SILT,3=SAND,4=GRAVEL,5=COBBLE,6=BOULDER,7=BEDROCK,8=OTHER)	NU	Sediment	TCEQ SOP V2	89844	GBRA
AVERAGE PERCENT OF SUBSTRATE GRAVEL SIZE OR LARGER	%	Other	TCEQ SOP V2	89845	GBRA
AVERAGE STREAM BANK EROSION (%)	%	Other	TCEQ SOP V2	89846	GBRA
AVERAGE STREAM BANK SLOPE (DEGREES)	deg	Other	TCEQ SOP V2	89847	GBRA
HABITAT FLOW STATUS, 1=NO FLOW, 2=LOW,3=MOD,4=HIGH	NU	Other	TCEQ SOP V2	89848	GBRA
AVERAGE PERCENT TREES AS RIPARIAN VEGETATION	%	Other	TCEQ SOP V2	89849	GBRA
AVERAGE PERCENT SHRUBS AS RIPARIAN VEGETATION	%	Other	TCEQ SOP V2	89850	GBRA
AVERAGE PERCENT GRASS AS RIPARIAN VEGETATION	%	Other	TCEQ SOP V2	89851	GBRA
AVERAGE PERCENT CULTIVATED FIELDS AS RIPARIAN VEGETATION	%	Other	TCEQ SOP V2	89852	GBRA
AVERAGE PERCENT OTHER AS RIPARIAN VEGETATION	%	Other	TCEQ SOP V2	89853	GBRA
AVERAGE PERCENTAGE OF TREE CANOPY COVERAGE	%	Other	TCEQ SOP V2	89854	GBRA
DRAINAGE AREA ABOVE MOST DOWNSTREAM TRANSECT*	km2	Other	TCEQ SOP V2	89859	GBRA
REACH LENGTH OF STREAM EVALUATED (M)	m	Other	NA/Calculation	89884	GBRA
AVERAGE STREAM WIDTH (METERS)	M	Other	TCEQ SOP V2	89861	GBRA
AVERAGE STREAM DEPTH (METERS)	M	Other	TCEQ SOP V2	89862	GBRA
MAXIMUM POOL WIDTH AT TIME OF STUDY (METERS)	M	Other	TCEQ SOP V2	89864	GBRA
MAXIMUM POOL DEPTH AT TIME OF STUDY(METERS)	M	Other	TCEQ SOP V2	89865	GBRA
AVERAGE WIDTH OF NATURAL RIPARIAN VEGETATION (M)	M	Other	TCEQ SOP V2	89866	GBRA
AVERAGE WIDTH OF NATURAL RIPARIAN BUFFER ON LEFT BANK (M)	M	Other	NA/Calculation	89872	GBRA
AVERAGE WIDTH OF NATURAL RIPARIAN BUFFER ON RIGHT BANK (M)	m	Other	NA/Calculation	89873	GBRA
AESTHETICS OF REACH(1=WILD 2=NAT. 3=COMM. 4=OFF.)	NU	Other	TCEQ SOP V2	89867	GBRA

NUMBER OF STREAM COVER TYPES	NU	Other	TCEQ SOP V2	89929	GBRA
LAND DEVELOP IMPACT (1=UNIMP,2=LOW,3=MOD,4=HIGH)	NU	Other	TCEQ SOP V2	89962	GBRA
RIPARIAN VEGETATION %; LEFT BANK - TREES	%	Other	NA/Calculation	89822	GBRA
RIPARIAN VEGETATION %; RIGHT BANK - TREES	%	Other	NA/Calculation	89823	GBRA
RIPARIAN VEGETATION %; LEFT BANK SHRUBS	%	Other	NA/Calculation	89824	GBRA
RIPARIAN VEGETATION %; RIGHT BANK - SHRUBS	%	Other	NA/Calculation	89825	GBRA
RIPARIAN VEGETATION %: LEFT BANK - GRASSES OR FORBS	%	Other	NA/Calculation	89826	GBRA
RIPARIAN VEGETATION %; RIGHT BANK - GRASSES OR FORBS	%	Other	NA/Calculation	89827	GBRA
RIPARIAN VEGETATION %: LEFT BANK - CULTIVATED FIELDS	%	Other	NA/Calculation	89828	GBRA
RIPARIAN VEGETATION %: RIGHT BANK - CULTIVATED FIELDS	%	Other	NA/Calculation	89829	GBRA
RIPARIAN VEGETATION %: LEFT BANK - OTHER	%	Other	NA/Calculation	89830	GBRA
RIPARIAN VEGETATION %: RIGHT BANK - OTHER	%	Other	NA/Calculation	89871	GBRA
AVAILABLE INSTREAM COVER HQI SCORE: 4=ABUNDANT 3=COMMON 2=RARE 1=ABSENT	NU	Other	NA/Calculation	89874	GBRA
BOTTOM SUBSTRATE STABILITY HQI SCORE: 4=STABLE 3=MODERATELY STABLE 2=MODERATELY UNSTABLE 1=UNSTABLE	NU	Other	NA/Calculation	89875	GBRA
NUMBER OF RIFFLES HQI SCORE: 4=ABUNDANT 3=COMMON 2=RARE 1=ABSENT	NS	Other	NA/Calculation	89876	GBRA
DIMENSIONS OF LARGEST POOL HQI SCORE: 4=LARGE 3=MODERATE 2=SMALL 1=ABSENT	NU	Other	NA/Calculation	89877	GBRA
CHANNEL FLOW STATUS HQI SCORE: 3=HIGH 2=MODERATE 1=LOW 0=NO FLOW	NU	Other	NA/Calculation	89878	GBRA
BANK STABILITY HQI SCORE: 3=STABLE 2=MODERATELY STABLE 1=MODERATELY UNSTABLE 0=UNSTABLE	NU	Other	NA/Calculation	89879	GBRA
CHANNEL SINUOSITY HQI SCORE: 3=HIGH 2=MODERATE 1=LOW 0=NONE	NU	Other	NA/Calculation	89880	GBRA
RIPARIAN BUFFER VEGETATION HQI SCORE: 3=EXTENSIVE 2=WIDE 1=MODERATE 0=NARROW	NU	Other	NA/Calculation	89881	GBRA
AESTHETICS OF REACH HQI SCORE: 3=WILDERNESS 2=NATURAL AREA 1=COMMON SETTING 0=OFFENSIVE	NU	Other	NA/Calculation	89882	GBRA

HQI TOTAL SCORE	NU	Other	NA/Calculation	89883	GBRA
LENGTH OF STREAM EVALUATED (KM)	KM	Other	NA/Calculation	89860	GBRA
STREAMBED SLOPE (FT/FT)	FT/FT	Other	NA/Calculation	72052	GBRA
NO FLOW ISOLATED POOL: LARGEST POOL MAX WIDTH (M)	M	Other	NA/Calculation	89908	GBRA
NO FLOW ISOLATED POOL: LARGEST POOL MAX LENGTH (M)	M	Other	NA/Calculation	89909	GBRA
NO FLOW ISOLATED POOL: LARGEST POOL MAX DEPTH (M)	M	Other	NA/Calculation	89910	GBRA
NO FLOW ISOLATED POOL: SMALLEST POOL MAX DEPTH (M)	M	Other	NA/Calculation	89911	GBRA
NO FLOW ISOLATED POOL: SMALLEST POOL MAX WIDTH (M)	M	Other	NA/Calculation	89912	GBRA
NO FLOW ISOLATED POOL: SMALLEST POOL MAX LENGTH (M)	M	Other	NA/Calculation	89913	GBRA
NO FLOW ISOLATED POOLS: NUMBER OF POOLS EVALUATED	NU	Other	NA/Calculation	89914	GBRA
<p>* From USGS map.</p> <p>References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415). TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).</p>					

TABLE A6.1g Measurement Performance Specifications for GBRA					
Biological - Benthics (Qualitative)					
Parameter	Units	Matrix	Method	Parameter Code	Lab
STREAM ORDER	NU	Water	TCEQ SOP, V1	84161	GBRA
BIOLOGICAL DATA	NS	Other	NA/Calculation	89888	GBRA
RAPID BIOASSESSMENT PROTOCOLS REGIONAL BENTHIC MACROINVERTEBRATE IBI SCORE	NS	Other	NA/Calculation	90082	GBRA
BENTHIC DATA REPORTING UNITS (1=NUMBER OF INDIVIDUALS IN SUB-SAMPLE, 2=NUMBER OF INDIVIDUALS/FT2, 3=NUMBER OF INDIVIDUALS/M2, 4=TOTAL NUMBER OF INDIVIDUALS IN SAMPLE)	NU	Other	TCEQ SOP V2	89899	GBRA

DIP NET EFFORT,AREA SWEPT (SQ.METER)	m2	Other	TCEQ SOP V2	89902	GBRA
KICKNET EFFORT,AREA KICKED (SQ.METER)	m2	Other	TCEQ SOP V2	89903	GBRA
KICKNET EFFORT,MINUTES KICKED (MIN.)	min.	Other	TCEQ SOP V2	89904	GBRA
DEBRIS/SHORELINE SAMPLING EFFORT, MINUTES	min.	Other	TCEQ SOP V2	89905	GBRA
NUMBER OF INDIVIDUALS IN BENTHIC SAMPLE	NU	Other	TCEQ SOP V2	89906	GBRA
UNDERCUT BANK AT COLLECTION POINT (%)	%	Other	TCEQ SOP V2	89921	GBRA
OVERHANGING BRUSH AT COLLECTION POINT (%)	%	Other	TCEQ SOP V2	89922	GBRA
GRAVEL BOTTOM AT COLLECTION POINT (%)	%	Sediment	TCEQ SOP V2	89923	GBRA
SAND BOTTOM AT COLLECTION POINT (%)	%	Sediment	TCEQ SOP V2	89924	GBRA
SOFT BOTTOM AT COLLECTION POINT (%)	%	Sediment	TCEQ SOP V2	89925	GBRA
MACROPHYTE BED AT COLLECTION POINT (%)	%	Other	TCEQ SOP V2	89926	GBRA
SNAGS AND BRUSH AT COLLECTION POINT (%)	%	Other	TCEQ SOP V2	89927	GBRA
BEDROCK STREAMBED AT COLLECTION POINT (%)	%	Sediment	TCEQ SOP V2	89928	GBRA
PETERSEN SAMPLER EFFORT, AREA SAMPLED (SQ. MTR.)	m2	Other	TCEQ SOP V2	89934	GBRA
EKMAN SAMPLER EFFORT, AREA SAMPLED (SQ.METER)	m2	Other	TCEQ SOP V2	89935	GBRA
MESH SIZE, ANY NET OR SIEVE, AVERAGE BAR (CM)	cm	Other	TCEQ SOP V2	89946	GBRA
BENTHIC SAMPLE COLLECTION METHOD (1=SURBER, 2=EKMAN, 3=KICKNET, 4=PETERSON, 5=HESTER DENDY, 6=SNAG, 7=HESS)	NU	Other	TCEQ SOP V2	89950	GBRA
ECOREGION LEVEL III (TEXAS Ecoregion Code)	NU	Other	TCEQ SOP V1	89961	GBRA
BENTHOS ORGANISMS -NONE PRESENT (0=NONE PRESENT)	NS	Other	TCEQ SOP V2	90005	GBRA
HILSENHOFF BIOTIC INDEX (HBI)	NU	Other	TCEQ SOP V2	90007	GBRA
NUMBER OF EPT INDEX	NU	Other	TCEQ SOP V2	90008	GBRA
DOMINANT BENTHIC FUNCTIONAL FEEDING GRP, % OF INDIVIDUALS	%	Other	TCEQ SOP V2	90010	GBRA
BENTHIC GATHERERS, PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	90025	GBRA
BENTHIC PREDATORS, PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	90036	GBRA
DOMINANT TAXON, BENTHOS PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	90042	GBRA

RATIO OF INTOLERANT TO TOLERANT TAXA, BENTHOS	NU	Other	TCEQ SOP V2	90050	GBRA
NUMBER OF NON-INSECT TAXA	NU	Other	TCEQ SOP V2	90052	GBRA
ELMIDAE, PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	90054	GBRA
TOTAL TAXA RICHNESS, BENTHOS	NU	Other	TCEQ SOP V2	90055	GBRA
CHIRONOMIDAE, PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	90062	GBRA
PERCENT OF TOTAL TRICHOPTERA INDIVIDUALS AS HYDROPSYCHIDAE	%	Other	TCEQ SOP V2	90069	GBRA
PERCENT EPHEMEROPTERA	%	Other	TCEQ SOP V2	91818	GBRA
PERCENT DIPTERA AND NON-INSECT TAXA	%	Other	TCEQ SOP V2	91814	GBRA
TOLERANT BENTHOS, PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	90066	GBRA
NUMBER OF EPHEMEROPTERA TAXA	%	Other	TCEQ SOP V2	90057	GBRA
TOTAL NUMBER OF INTOLERANT TAXA, BENTHOS	%	Other	TCEQ SOP V2	90058	GBRA
BENTHIC SCRAPERS, PERCENT OF INDIVIDUALS	%	Other	TCEQ SOP V2	91815	GBRA
TOTAL # OF BENTHIC GENERA IN SAMPLE	NU	Other	TCEQ SOP V2	90011	GBRA
BENTHIC SHREDDERS (% OF COMMUNITY)	%	Other	TCEQ SOP V2	90035	GBRA
HESS SAMPLER EFFORT, AREA SAMPLED (SQ. METER)	m2	Other	TCEQ SOP V2	89956	GBRA
References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415). TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).					

TABLE A6.1h Measurement Performance Specifications for GBRA					
Biological - Nekton					
Parameter	Units	Matrix	Method	Parameter Code	Lab
STREAM ORDER	NU	Water	TCEQ SOP V1	84161	GBRA

NEKTON TEXAS REGIONAL IBI SCORE	NS	Other	NA/Calculation	98123	GBRA
BIOLOGICAL DATA	NS	Other	NA/Calculation	89888	GBRA
SEINE, MINIMUM MESH SIZE, AVERAGE BAR, NEKTON,IN	IN	Other	TCEQ SOP V2	89930	GBRA
SEINE, MAXIMUM MESH SIZE, AVG BAR, NEKTON,INCH	IN	Other	TCEQ SOP V2	89931	GBRA
NET LENGTH (METERS)	M	Other	TCEQ SOP V2	89941	GBRA
ELECTROFISHING METHOD 1=BOAT 2=BACKPACK 3=TOTE BARGE	NU	Other	TCEQ SOP V2	89943	GBRA
ELECTROFISH EFFORT, DURATION OF SHOCKING (SEC)	SEC	Other	TCEQ SOP V2	89944	GBRA
SEINING EFFORT (# OF SEINE HAULS)	NU	Other	TCEQ SOP V2	89947	GBRA
COMBINED LENGTH OF SEINE HAULS (METERS)	M	Other	TCEQ SOP V2	89948	GBRA
SEINING EFFORT, DURATION (MINUTES)	MIN	Other	TCEQ SOP V2	89949	GBRA
ECOREGION LEVEL III (TEXAS Ecoregion Code)	NU	Other	TCEQ SOP V1	89961	GBRA
AREA SEINED (SQ METERS)	M2	Other	TCEQ SOP V2	89976	GBRA
NUMBER OF SPECIES, FISH	NU	Other	TCEQ SOP V2	98003	GBRA
NEKTON ORGANISMS-NONE PRESENT (0=NONE PRESENT)	NS	Other	TCEQ SOP V2	98005	GBRA
TOTAL NUMBER OF SUNFISH SPECIES	NU	Other	TCEQ SOP V2	98008	GBRA
TOTAL NUMBER OF INTOLERANT SPECIES, FISH	NU	Other	TCEQ SOP V2	98010	GBRA
PERCENT OF INDIVIDUALS AS OMNIVORES, FISH	%	Other	TCEQ SOP V2	98017	GBRA
PERCENT OF INDIVIDUALS AS INVERTIVORES, FISH	%	Other	TCEQ SOP V2	98021	GBRA
PERCENT OF INDIVIDUALS AS PISCIVORES, FISH	%	Other	TCEQ SOP V2	98022	GBRA
PERCENT OF INDIVIDUALS WITH DISEASE OR ANOMALY	%	Other	TCEQ SOP V2	98030	GBRA
TOTAL NUMBER OF NATIVE CYPRINID SPECIES	NU	Other	TCEQ SOP V2	98032	GBRA
PERCENT INDIVIDUALS AS NON-NATIVE FISH SPECIES (% OF COMMUNITY)	%	Other	TCEQ SOP V2	98033	GBRA
TOTAL NUMBER OF INDIVIDUALS SEINING	NU	Other	TCEQ SOP V2	98039	GBRA
TOTAL NUMBER OF INDIVIDUALS ELECTROFISHING	NU	Other	TCEQ SOP V2	98040	GBRA
TOTAL NUMBER OF BENTHIC INVERTIVORE SPECIES	NU	Other	TCEQ SOP V2	98052	GBRA

NUMBER OF INDIVIDUALS PER SEINE HAUL	NU	Other	TCEQ SOP V2	98062	GBRA
NUMBER OF INDIVIDUALS PER MINUTE ELECTROFISHING	NU	Other	TCEQ SOP V2	98069	GBRA
PERCENT INDIVIDUALS AS TOLERANT FISH SPECIES (EXCLUDING WESTERN MOSQUITOFISH)	%	Other	TCEQ SOP V2	98070	GBRA
TOTAL NUMBER OF INDIVIDUALS IN SAMPLE, FISH	NU	Other	TCEQ SOP V2	98023	GBRA
TOTAL NUMBER OF INDIVIDUALS IN SAMPLE, FISH	NU	Other	TCEQ SOP V2	98023	GBRA
PERCENT OF INDIVIDUALS AS INVERTIVORES, FISH	%	Other	TCEQ SOP V2	98021	GBRA
PERCENT OF INDIVIDUALS AS TOLERANTS, FISH	%	Other	TCEQ SOP V2	98016	GBRA
References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415). TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).					

TABLE A6.2a Measurement Performance Specifications for UGRA

Field Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
TEMPERATURE, WATER (DEGREES CENTIGRADE)	DEG C	water	SM 2550 B and TCEQ SOP V1	00010	UGRA Field
TRANSPARENCY, SECCHI DISC (METERS)**	meters	water	TCEQ SOP V1	00078	UGRA Field
SPECIFIC CONDUCTANCE, FIELD (US/CM @ 25C)	us/cm	water	EPA 120.1 and TCEQ SOP, V1	00094	UGRA Field
OXYGEN, DISSOLVED (MG/L)	mg/L	water	SM 4500-O G and TCEQ SOP V1	00300	UGRA Field
PH (STANDARD UNITS)	s.u	water	EPA 150.1 and TCEQ SOP V1	00400	UGRA Field
DAYS SINCE PRECIPITATION EVENT (DAYS)	days	other	TCEQ SOP V1	72053	UGRA Field
DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE*	meters	water	TCEQ SOP V2	82903	UGRA Field

MAXIMUM POOL WIDTH AT TIME OF STUDY (METERS)*	meters	other	TCEQ SOP V2	89864	UGRA Field
MAXIMUM POOL DEPTH AT TIME OF STUDY(METERS)*	meters	other	TCEQ SOP V2	89865	UGRA Field
POOL LENGTH, METERS*	meters	other	TCEQ SOP V2	89869	UGRA Field
% POOL COVERAGE IN 500 METER REACH*	%	other	TCEQ SOP V2	89870	UGRA Field
<p>* To be routinely reported when collecting data from perennial pools. ** Transparency only sampled quarterly at stations 15111 and 15113</p> <p>References: United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415). TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).</p>					

TABLE A6.2b Measurement Performance Specifications for UGRA					
Flow Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
FLOW STREAM, INSTANTANEOUS (CUBIC FEET PER SEC)	cfs	water	TCEQ SOP V1	00061	UGRA Field
FLOW SEVERITY: 1=No Flow,2=Low,3=Normal,4=Flood,5=High,6=Dry	NU	water	TCEQ SOP V1	01351	UGRA Field
STREAM FLOW ESTIMATE (CFS)*	cfs	Water	TCEQ SOP V1	74069	UGRA Field
FLOW MTH 1=GAGE 2=ELEC 3=MECH 4=WEIR/FLU 5=DOPPLER	NU	other	TCEQ SOP V1	89835	UGRA Field
*In cases where a direct flow measurement may not be possible and there are no USGS flow gages representative of conditions at the monitoring site, discharge data from the nearest flow gage is					

submitted as a flow estimate. See Table B1.1.

References:

TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).

TABLE A6.2c Measurement Performance Specifications for UGRA

Conventional Parameters in Water

Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Precision (RPD)	Bias %Rec. of LCS	Lab
RESIDUE, TOTAL NONFILTRABLE (MG/L)	mg/L	water	SM 2540D	00530	5	1*	NA	NA	NA	UGRA, GBRA, and SPL, and SARA-REL **
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	Mg/L	Water	SM 4500-NH3 D	00610	0.1	0.1	70-130	20	80-120	UGRA and SARA-REL **
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	EPA 350.1 Rev. 2.0 (1993)	00610	0.1	0.1	70-130	20	80-120	GBRA and SPL**
NITRATE NITROGEN, TOTAL (MG/L AS N)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00620	0.05	0.04	70-130	20	80-120	UGRA**
NITRATE NITROGEN, TOTAL (MG/L AS N)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	620	0.05	0.05	70-130	20	80-120	GBRA, SPL, SARA-REL**
NITROGEN, KJELDAHL, TOTAL (MG/L AS N)	mg/L	water	EPA 351.2 Rev. 2 (1993)	00625	0.2	0.2	70-130	20	80-120	GBRA, SPL, SARA-REL ***
PHOSPHORUS, TOTAL, WET METHOD (MG/L AS P)	mg/L	water	SM 4500-P E.	00665	0.06	0.05	70-130	20	80-120	UGRA**
PHOSPHORUS, TOTAL, WET METHOD (MG/L AS P)	mg/L	water	EPA 365.3	00665	0.06	0.02	70-130	20	80-120	GBRA, SPL, SARA-REL**
CHLORIDE (MG/L AS CL)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00940	5	0.2	70-130	20	80-120	UGRA**

CHLORIDE (MG/L AS CL)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00940	5	1	70-130	20	80-120	GBRA, SPL **
CHLORIDE (MG/L AS CL)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00940	5	5	70-130	20	80-120	SARA-REL **
SULFATE (MG/L AS SO4)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00945	5	0.2	70-130	20	80-120	UGRA**
SULFATE (MG/L AS SO4)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00945	5	1	70-130	20	80-120	GBRA, SPL **
SULFATE (MG/L AS SO4)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00945	5	5	70-130	20	80-120	SARA-REL**
CHLOROPHYLL-A UG/L SPECTROPHOTOMETRIC ACID. METH	ug/L	water	SM 10200-H4	32211	3	1	NA	20	80-120	GBRA***
CHLOROPHYLL-A UG/L SPECTROPHOTOMETRIC ACID. METH	ug/L	water	SM 10200-H	32211	3	1	NA	20	80-120	SARA-REL***
CHLOROPHYLL-A, FLUOROMETRIC METHOD, UG/L	µg/L	water	EPA 445.0	70953	3	1	NA	20	80-120	SPL ***
PHEOPHYTIN-A UG/L SPECTROPHOTOMETRIC ACID. METH.	µg/L	water	SM 10200-H4	32218	3	1	NA	NA	NA	GBRA***
PHEOPHYTIN-A UG/L SPECTROPHOTOMETRIC ACID. METH.	µg/L	water	SM 10200-H	32218	3	1	NA	NA	NA	SARA-REL***
PHEOPHYTIN-A UG/L FLUOROMETRIC METHOD	µg/L	Water	EPA 445	32213	3	1	NA	NA	NA	SPL ***
TURBIDITY,LAB NEPHELOMETRIC TURBIDITY UNITS, NTU	NTU	water	SM 2130B	82079	0.5	0.5	NA	NA	NA	UGRA, GBRA, SPL**
TURBIDITY,LAB NEPHELOMETRIC TURBIDITY UNITS, NTU	NTU	water	EPA 180.1	82079	0.5	0.5	NA	NA	NA	SARA-REL**

*TSS LOQ is based on the volume of sample used.

**GBRA, SPL, or SARA-REL will be used in the event of an equipment failure and the need to meet holding times.

***GBRA is the primary laboratory for this parameter. SARA-REL Laboratory or SPL will be used in the event of a GBRA equipment failure and the need to meet holding times

References:

United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods

Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version

TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).

TABLE A6.2d Measurement Performance Specifications for UGRA

Bacteriological Parameters in Water

Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Log Difference of Duplicates	Bias %Rec. of LCS	Lab
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	IDEXX Laboratories Colilert®-18**	31699	1	1	NA	0.50*	NA	GBRA***
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	SM 9223-B**	31699	1	1	NA	0.50*	NA	UGRA, SPL, SARA-REL ***
E.COLI, COLILERT, IDEXX, HOLDING TIME	hours	water	NA	31704	NA	NA	NA	NA	NA	UGRA, GBRA, SPL, SARA-REL ***

* This value is not expressed as a relative percent difference. It represents the maximum allowable difference between the logarithm of the result of a sample and the logarithm of the duplicate result. See Section B4.

** *E.coli* samples analyzed by these methods should always be processed as soon as possible and within 8 hours. When transport conditions necessitate delays in delivery longer than 6 hours, the holding time may be extended and samples must be processed as soon as possible and within 30 hours.

***GBRA Laboratory, SPL, or SARA-REL will be used in the event of an equipment failure and the need to meet holding times.

References:

Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version

Annual Book of ASTM Standards, Section 11, Water and Environmental Technology, Volume 11.02, Water

TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).

TABLE A6.2e Measurement Performance Specifications for UGRA					
24 Hour Parameters in Water					
Parameter	Units	Matrix	Method	Parameter Code	Lab
TEMPERATURE, WATER (DEGREES CENTIGRADE), 24HR AVG	DEG C	Water	TCEQ SOP V1	00209	UGRA field
WATER TEMPERATURE, DEGREES CENTIGRADE, 24HR MAX	DEG C	Water	TCEQ SOP V1	00210	UGRA field
TEMPERATURE, WATER (DEGREES CENTIGRADE) 24HR MIN	DEG C	Water	TCEQ SOP V1	00211	UGRA field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR AVG	uS/cm	Water	TCEQ SOP V1	00212	UGRA field

SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR MAX	uS/cm	Water	TCEQ SOP V1	00213	UGRA field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR MIN	uS/cm	Water	TCEQ SOP V1	00214	UGRA field
PH, S.U., 24HR MAXIMUM VALUE	std. units	Water	TCEQ SOP V1	00215	UGRA field
PH, S.U., 24HR, MINIMUM VALUE	std. units	Water	TCEQ SOP V1	00216	UGRA field
WATER TEMPERATURE, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00221	UGRA field
SPECIFIC CONDUCTANCE, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00222	UGRA field
pH, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00223	UGRA field
DISSOLVED OXYGEN, 24-HOUR MIN. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89855	UGRA field
DISSOLVED OXYGEN, 24-HOUR MAX. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89856	UGRA field
DISSOLVED OXYGEN, 24-HOUR AVG. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89857	UGRA field
DISSOLVED OXYGEN, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	89858	UGRA field
References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).					

TABLE A6.3a Measurement Performance Specifications for MCWE					
Field Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab

TEMPERATURE, WATER (DEGREES CENTIGRADE)	DEG C	water	SM 2550 B and TCEQ SOP V1	00010	MCWE Field
TRANSPARENCY, SECCHI DISC (METERS)**	meters	water	TCEQ SOP V1	00078	MCWE Field
SPECIFIC CONDUCTANCE, FIELD (US/CM @ 25C)	us/cm	water	EPA 120.1 and TCEQ SOP, V1	00094	MCWE Field
OXYGEN, DISSOLVED (MG/L)	mg/L	water	SM 4500-O G and TCEQ SOP V1	00300	MCWE Field
PH (STANDARD UNITS)	s.u	water	EPA 150.1 and TCEQ SOP V1	00400	MCWE Field
DAYS SINCE PRECIPITATION EVENT (DAYS)	days	other	TCEQ SOP V1	72053	MCWE Field
DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE	meters	water	TCEQ SOP V2	82903	MCWE Field
MAXIMUM POOL WIDTH AT TIME OF STUDY (METERS)*	meters	other	TCEQ SOP V2	89864	MCWE Field
MAXIMUM POOL DEPTH AT TIME OF STUDY(METERS)*	meters	other	TCEQ SOP V2	89865	MCWE Field
POOL LENGTH, METERS*	meters	other	TCEQ SOP V2	89869	MCWE Field
% POOL COVERAGE IN 500 METER REACH*	%	other	TCEQ SOP V2	89870	MCWE Field
<p>* To be routinely reported when collecting data from perennial pools. ** Transparency sampled at all MCWE stations</p> <p>References: United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415). TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).</p>					

TABLE A6.3b Measurement Performance Specifications for MCWE

Flow Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
FLOW STREAM, INSTANTANEOUS (CUBIC FEET PER SEC)	cfs	water	TCEQ SOP V1	00061	MCWE Field
FLOW SEVERITY: 1=No Flow,2=Low,3=Normal,4=Flood,5=High,6=Dry	NU	water	TCEQ SOP V1	01351	MCWE Field
STREAM FLOW ESTIMATE (CFS)*	cfs	Water	TCEQ SOP V1	74069	MCWE Field
FLOW MTH 1=GAGE 2=ELEC 3=MECH 4=WEIR/FLU 5=DOPPLER	NU	other	TCEQ SOP V1	89835	MCWE Field
<p>*In cases where a direct flow measurement may not be possible and there are no USGS flow gages representative of conditions at the monitoring site, discharge data from the nearest flow gage is submitted as a flow estimate. See Table B1.1.</p> <p>References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).</p>					

TABLE A6.3c Measurement Performance Specifications for MCWE										
Conventional Parameters in Water										
Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Precision (RPD)	Bias %Rec. of LCS	Lab
RESIDUE, TOTAL NONFILTRABLE (MG/L)	mg/L	water	SM 2540D	00530	5	1*	NA	NA	NA	GBRA, SPL, SARA-REL **
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	EPA 350.1 Rev. 2.0 (1993)	00610	0.1	0.1	70-130	20	80-120	GBRA and SPL **
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	SM 4500 NH3D	00610	0.1	0.1	70-130	20	80-120	SARA-REL **
NITRATE NITROGEN, TOTAL (MG/L AS N)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00620	0.05	0.05	70-130	20	80-120	GBRA, SPL, and SARA-REL **

PHOSPHORUS, TOTAL, WET METHOD (MG/L AS P)	mg/L	water	EPA 365.3	00665	0.06	0.02	70-130	20	80-120	GBRA, SPL, SARA-REL **
<p>*TSS LOQ is based on the volume of sample used. **GBRA Laboratory is the primary lab. SPL or SARA-REL will be used in the event of an equipment failure and the need to meet holding times.</p> <p>References: United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).</p>										

TABLE A6.3d Measurement Performance Specifications for MCWE										
Bacteriological Parameters in Water										
Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Log Difference of Duplicates	Bias %Rec. of LCS	Lab
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	IDEXX Laboratories Colilert®-18**	31699	1	1	NA	0.50*	NA	GBRA ***
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	SM 9223-B IDEXX**	31699	1	1	NA	0.50*	NA	SPL, SARA-REL ***
E.COLI, COLILERT, IDEXX, HOLDING TIME	hours	water	NA	31704	NA	NA	NA	NA	NA	GBRA, SPL, and SARA-REL***
<p>* This value is not expressed as a relative percent difference. It represents the maximum allowable difference between the logarithm of the result of a sample and the logarithm of the duplicate result. See Section B4. ** <i>E.coli</i> samples analyzed by these methods should always be processed as soon as possible and within 8 hours. When transport conditions necessitate delays in delivery longer than 6 hours, the holding time may be extended and samples must be processed as soon as possible and within 30 hours. *** GBRA Laboratory is the primary lab. SPL or SARA-REL will be used in the event of an equipment failure and the need to meet holding times.</p> <p>References: Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version Annual Book of ASTM Standards, Section 11, Water and Environmental Technology, Volume 11.02, Water TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).</p>										

TABLE A6.3e Measurement Performance Specifications for MCWE
24 Hour Parameters in Water

Parameter	Units	Matrix	Method	Parameter Code	Lab
TEMPERATURE, WATER (DEGREES CENTIGRADE), 24HR AVG	DEG C	Water	TCEQ SOP V1	00209	MCWE field
WATER TEMPERATURE, DEGREES CENTIGRADE, 24HR MAX	DEG C	Water	TCEQ SOP V1	00210	MCWE field
TEMPERATURE, WATER (DEGREES CENTIGRADE) 24HR MIN	DEG C	Water	TCEQ SOP V1	00211	MCWE field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR AVG	uS/cm	Water	TCEQ SOP V1	00212	MCWE field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR MAX	uS/cm	Water	TCEQ SOP V1	00213	MCWE field
SPECIFIC CONDUCTANCE, US/CM, FIELD, 24HR MIN	uS/cm	Water	TCEQ SOP V1	00214	MCWE field
PH, S.U., 24HR MAXIMUM VALUE	std. units	Water	TCEQ SOP V1	00215	MCWE field
PH, S.U., 24HR, MINIMUM VALUE	std. units	Water	TCEQ SOP V1	00216	MCWE field
WATER TEMPERATURE, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00221	MCWE field
SPECIFIC CONDUCTANCE, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00222	MCWE field
pH, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	00223	MCWE field
DISSOLVED OXYGEN, 24-HOUR MIN. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89855	MCWE field
DISSOLVED OXYGEN, 24-HOUR MAX. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89856	MCWE field
DISSOLVED OXYGEN, 24-HOUR AVG. (MG/L) MIN. 4 MEA	mg/l	Water	TCEQ SOP V1	89857	MCWE field
DISSOLVED OXYGEN, # OF MEASUREMENTS IN 24-HRS	NU	Water	TCEQ SOP V1	89858	MCWE field
References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).					

TABLE A6.4a Measurement Performance Specifications for HZ

Field Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
TEMPERATURE, WATER (DEGREES CENTIGRADE)	DEG C	water	SM 2550 B and TCEQ SOP V1	00010	HZ Field
TRANSPARENCY, SECCHI DISC (METERS)**	meters	water	TCEQ SOP V1	00078	HZ Field
SPECIFIC CONDUCTANCE, FIELD (US/CM @ 25C)	us/cm	water	EPA 120.1 and TCEQ SOP, V1	00094	HZ Field
OXYGEN, DISSOLVED (MG/L)	mg/L	water	SM 4500-O G and TCEQ SOP V1	00300	HZ Field
PH (STANDARD UNITS)	s.u	water	EPA 150.1 and TCEQ SOP V1	00400	HZ Field
DAYS SINCE PRECIPITATION EVENT (DAYS)	days	other	TCEQ SOP V1	72053	HZ Field
DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE	meters	water	TCEQ SOP V2	82903	HZ Field
MAXIMUM POOL WIDTH AT TIME OF STUDY (METERS)*	meters	other	TCEQ SOP V2	89864	HZ Field
MAXIMUM POOL DEPTH AT TIME OF STUDY(METERS)*	meters	other	TCEQ SOP V2	89865	HZ Field
POOL LENGTH, METERS*	meters	other	TCEQ SOP V2	89869	HZ Field
% POOL COVERAGE IN 500 METER REACH*	%	other	TCEQ SOP V2	89870	HZ Field
<p>* To be routinely reported when collecting data from perennial pools. ** Transparency sampled at all HZ stations</p> <p>References: United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415). TCEQ SOP, V2 - TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data, 2014 (RG-416).</p>					

TABLE A6.4b Measurement Performance Specifications for HZ					
Flow Parameters					
Parameter	Units	Matrix	Method	Parameter Code	Lab
FLOW STREAM, INSTANTANEOUS (CUBIC FEET PER SEC)	cfs	water	TCEQ SOP V1	00061	HZ Field
FLOW SEVERITY: 1=No Flow,2=Low,3=Normal,4=Flood,5=High,6=Dry	NU	water	TCEQ SOP V1	01351	HZ Field
STREAM FLOW ESTIMATE (CFS)*	cfs	Water	TCEQ SOP V1	74069	HZ Field
FLOW MTH 1=GAGE 2=ELEC 3=MECH 4=WEIR/FLU 5=DOPPLER	NU	other	TCEQ SOP V1	89835	HZ Field
<p>*In cases where a direct flow measurement may not be possible and there are no USGS flow gages representative of conditions at the monitoring site, discharge data from the nearest flow gage is submitted as a flow estimate. See Table B1.1.</p> <p>References: TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).</p>					

TABLE A6.4c Measurement Performance Specifications for HZ										
Conventional Parameters in Water										
Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Precision (RPD)	Bias %Rec. of LCS	Lab
RESIDUE, TOTAL NONFILTRABLE (MG/L)	mg/L	water	SM 2540D	00530	5	1*	NA	NA	NA	GBRA, SPL, SARA-REL**
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	EPA 350.1 Rev. 2.0 (1993)	00610	0.1	0.1	70-130	20	80-120	GBRA and SPL**
NITROGEN, AMMONIA, TOTAL (MG/L AS N)	mg/L	water	SM 4500 NH3D	00610	0.1	0.1	70-130	20	80-120	SARA-REL**
NITRATE NITROGEN, TOTAL (MG/L AS N)	mg/L	water	EPA 300.0 Rev. 2.1 (1993)	00620	0.05	0.05	70-130	20	80-120	GBRA, SPL, SARA-REL**

NITROGEN, KJELDAHL, TOTAL (MG/L AS N)	mg/L	water	EPA 351.2 Rev. 2 (1993)	00625	0.2	0.2	70-130	20	80-120	GBRA, SPL, SARA-REL **
PHOSPHORUS, TOTAL, WET METHOD (MG/L AS P)	mg/L	water	EPA 365.3	00665	0.06	0.02	70-130	20	80-120	GBRA, SPL, SARA-REL **

*TSS LOQ is based on the volume of sample used.
 **GBRA Laboratory is the primary lab. SPL or SARA-REL will be used in the event of an equipment failure and the need to meet holding times.

References:
 United States Environmental Protection Agency (USEPA), Clean Water Act Analytical Methods Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version
 TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).

TABLE A6.4d Measurement Performance Specifications for HZ										
Bacteriological Parameters in Water										
Parameter	Units	Matrix	Method	Parameter Code	TCEQ AWRL	LOQ	LOQ Check Sample %Rec	Log Difference of Duplicates	Bias %Rec. of LCS	Lab
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	IDEXX Laboratories Colilert®-18**	31699	1	1	NA	0.50*	NA	GBRA***
E. COLI, COLILERT, IDEXX METHOD, MPN/100ML	MPN/100 mL	water	SM 9223-B**	31699	1	1	NA	0.50*	NA	SPL, SARA-REL ***
E.COLI, COLILERT, IDEXX, HOLDING TIME	hours	water	NA	31704	NA	NA	NA	NA	NA	GBRA, SPL, SARA-REL ***

* This value is not expressed as a relative percent difference. It represents the maximum allowable difference between the logarithm of the result of a sample and the logarithm of the duplicate result. See Section B5.
 ** *E.coli* samples analyzed by these methods should always be processed as soon as possible and within 8 hours. When transport conditions necessitate delays in delivery longer than 6 hours, the holding time may be extended and samples must be processed as soon as possible and within 30 hours.
 *** GBRA Laboratory is the primary lab. SPL or SARA-REL will be used in the event of an equipment failure and the need to meet holding times.

References:
 Standard Methods for the Examination of Water and Wastewater, 24th Edition, 2022 or applicable version
 Annual Book of ASTM Standards, Section 11, Water and Environmental Technology, Volume 11.02, Water
 TCEQ SOP, V1 - TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods, 2012 (RG-415).

Appendix B: Task 3 Work Plan & Sampling Process Design and Monitoring Schedule (Plan)

Task 3: Water Quality Monitoring

Objectives: Water quality monitoring will focus on the characterization of a variety of locations and conditions. This will include a combination of the following:

- Planning and coordinating basin-wide monitoring.
- Routine, regularly scheduled monitoring to collect long-term information and support statewide assessment of water quality.
- Systematic, regularly scheduled short-term monitoring to screen water bodies for issues.

Task Description: The Performing Party will conduct water quality monitoring and provide details in the Quarterly Progress Report as prescribed in the FY 2026-2027 Guidance. The actual number of sites, location, frequency, and parameters collected will be based on priorities identified at the basin Steering Committee Meeting and Coordinated Monitoring meetings and included in the Appendix B schedule of the QAPP.

The Performing Party will complete the following subtasks:

Monitoring Description - In FY 2026, the Performing Party will conduct routine monitoring at a minimum of nineteen sites monthly and a minimum of thirteen sites quarterly for field, conventional, flow (at stream sites), and bacteria parameter groups. Biological and habitat monitoring events will be conducted at a minimum of one site in the Performing Party's basin. In addition, the Performing Party will coordinate with the Upper Guadalupe River Authority (UGRA) for the monitoring of a minimum of ten sites quarterly in Kerr County and one site quarterly in Kendall County for field, conventional, flow (at stream sites), and bacteria parameter groups. In FY 2027, the Performing Party will monitor at a similar level of effort as in FY 2026. The actual number of sites, location, frequency, and parameters collected in FY 2026 will be included in the Performing Party QAPP Appendix B update. All monitoring will be completed in accordance with the Performing Party QAPP, the *TCEQ Surface Water Quality Monitoring Procedures, Volume 1: Physical and Chemical Monitoring Methods* (RG-415) and the *TCEQ Surface Water Quality Monitoring Procedures, Volume 2: Methods for Collecting and Analyzing Biological Assemblage and Habitat Data* (RG-416).

Coordinated Monitoring Meeting - The Performing Party will hold an annual coordinated monitoring meeting as described in the FY2026-2027 CRP Guidance. Qualified monitoring organizations will be invited to attend the working meeting in which monitoring needs and purposes will be discussed segment by segment and station by station. Information from participants and stakeholders will be used to select stations and parameters that will enhance overall water quality monitoring coverage, eliminate duplication of effort, and address basin priorities. A summary of the changes to the monitoring schedule will be provided to the participants within two weeks of the meeting. Changes to the monitoring schedule will be entered into the statewide CMS (<http://cms.lcra.org>) and communicated to meeting attendees. Changes to monitoring schedules that occur during the year will be entered into the CMS and communicated to meeting attendees. All requirements related to meetings will be followed and required meetings will be conducted in-person or via TCEQ approved virtual format.

Monitoring Activities - Each progress report will include a description of activities including all types of monitoring performed, number of sampling events, and the types of monitoring conducted in the quarter. The Performing Party will complete and submit a monitoring activities report as an attachment to the progress report.

Deliverables and Due Dates:

September 1, 2025 through August 31, 2026

- A. Conduct water quality monitoring, submit monitoring activities report, summarize activities, and submit with progress report – December 15, 2025; March 15 and June 15, 2026
- B. Coordinated Monitoring Meeting – between March 15 and April 30, 2026
- C. Coordinated Monitoring Meeting Summary of Changes – within 2 weeks of the meeting
- D. Email notification that Coordinated Monitoring Schedule updates are complete – May 31, 2026

September 1, 2026 through August 31, 2027

- A. Conduct water quality monitoring, submit monitoring activities report, summarize activities, and submit with progress report – September 15 and December 15, 2026; March 15 and June 15 and August 15, 2027
- B. Coordinated Monitoring Meeting – between March 15 and April 30, 2027
- C. Coordinated Monitoring Meeting Summary of Changes – within 2 weeks of the meeting
- D. Email notification that Coordinated Monitoring Schedule updates are complete – May 31, 2027

Sample Design Rationale FY 2026

The sample design is based on the legislative intent of CRP. Under the legislation, the Basin Planning Agencies have been tasked with providing data to characterize water quality conditions in support of the Texas Integrated Report of Surface Water Quality, and to identify significant long-term water quality trends. Based on Steering Committee input, achievable water quality objectives and priorities and the identification of water quality issues are used to develop work plans which are in accord with available resources. As part of the Steering Committee process, GBRA coordinates closely with the TCEQ and other participants to ensure a comprehensive water monitoring strategy within the watershed. Although the Guadalupe River basin has overall good water quality, impacts from urbanization, agricultural runoff, and other factors may degrade water quality. Comprehensive water quality monitoring is therefore critical for identifying water quality problems and monitoring known issues. In addition, water quality monitoring is more critical than ever as this river basin experiences rapid population growth.

The following changes have been proposed to the monitoring schedule for FY2026. These changes have come about because of concerns or requests of steering committee members or monitoring entities at the annual Guadalupe River Basin Coordinated Monitoring Meeting.

1. GBRA will remove one ALM event at station 12678 (Johnson Creek at SH 39 in Ingram) on segment 1816 in FY26. One ALM event at station 12678 will occur during the critical period during FY26 since flooding/extreme scouring prevented sampling this in FY25.
2. Ammonia-nitrogen will be added to conventionals to be sampled by UGRA at station 12678 in FY26.
3. GBRA will conduct an ALM event at station 12681 (North Fork Guadalupe River at FM 1340) on

segment 1817. This event will consist of Aquatic Habitat, Benthic, Nekton, Field, and Flow monitoring at a frequency of two times per year in FY26. UGRA will collect 24 hour DO data and conventional samples for this event.

4. Hays County will replace the Watershed Association (WV) as the collecting entity for all associated stations on segment 1813 beginning in FY26.

5. Ammonia-nitrogen will be removed from the list of conventionals analyzed at station 12684 (South Fork Guadalupe Adjacent to Hunt Lions Park).

Site Selection Criteria

This data collection effort involves monitoring routine water quality using procedures that are consistent with the TCEQ SWQM program. Some general guidelines are followed when selecting sampling sites, as outlined below, and discussed thoroughly in SWQM Procedures, Volumes I and II. Overall consideration is given to accessibility and safety. All monitoring activities have been developed in coordination with the CRP Steering Committee and with the TCEQ. The site selection criteria specified are those the TCEQ would like considered to produce data which is complementary to that collected by the state and which may be used in assessments, etc.

1. Locate stream sites so that samples can be safely collected from the centroid of flow. Centroid is defined as the midpoint of that portion of stream width which contains 50 percent of the total flow. If multiple potential sites on a stream segment are appropriate for monitoring, choose one that would best represent the water body, and not a site that displays unusual conditions or contaminant source(s). Avoid backwater areas or eddies when selecting a stream site.
2. At a minimum for reservoirs, locate sites near the dam (reservoirs) and in the major arms. Larger reservoirs might also include stations in the middle and upper (riverine) areas. Select sites that best represent the water body by avoiding coves and back water areas. A single monitoring site is considered representative of 25 percent of the total reservoir acres, but not more than 5,120 acres.
3. Monitoring sites are selected to maximize stream coverage or basin coverage. Very long segments may require more stations. As a rule of thumb, stream segments between 25 and 50 miles long require two stations, and longer than 50 miles require three or more depending on the existence of areas with significantly different sources of contamination or potential water quality concerns. Major hydrological features, such as the confluence of a major tributary or an instream dam, may also limit the spatial extent of an assessment based on one station.
4. Because historical water quality data can be very useful in assessing use attainment or impairment, it may be best to use sites that are on current or past monitoring schedules.
5. All classified segments (including reservoirs) should have at least one Monitoring site that adequately characterizes the water body, and monitoring should be coordinated with the TCEQ or other qualified monitoring entities reporting routine data to TCEQ.
6. Monitoring sites may be selected to bracket sources of pollution, influence of tributaries, changes in land uses, and hydrological modifications.
7. Sites should be accessible. When possible, stream sites should have a USGS or IBWC stream flow gauge. If not, it should be possible to conduct flow measurement during routine visits.

Monitoring Sites for FY 2026

Table B1.1 Sample Design and Schedule, FY 2026

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
GUADALUPE RIVER AT LOWER GUADALUPE DIVERSION DAM AND SALT WATER BARRIER	12578	1802	14	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon
GUADALUPE RIVER AT FM 447 WEST OF NURSERY AND UPSTREAM OF SOUTH TEXAS ELECTRIC	12590	1803	14	GB	GB	RT									4			4	4		4	flow estimate taken from USGS gage 08176500
GUADALUPE RIVER AT OLD SAN ANTONIO ROAD/FM766 WEST OF CUERO	12592	1803	14	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon, flow estimate taken from USGS gage 08175800
GUADALUPE RIVER AT US 183 IN HOCHHEIM IN DEWITT COUNTY	20470	1803	14	GB	GB	RT									4			4	4		4	
ELM CREEK ON LAZY F RANCH 515 METERS UPSTREAM OF OLD US 87 BRIDGE	17894	1803A	14	GB	GB	RT									4			4	4		4	Routine Monitoring Added in FY20 to Confirm DO Impairment
SANDIES CREEK 100 FT DOWNSTREAM OF COUNTY HIGHWAY 1.9 MI UPSTREAM FROM BIRDS CREEK 2.0 MI NE OF WESTHOFF	13657	1803B	14	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon;

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
PEACH CREEK AT GONZALES CR 353 14.0KM EAST OF GONZALES	14937	1803C	14	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon, flow estimate taken from USGS gage 08174600
GUADALUPE RIVER 200 METERS DOWNSTREAM OF H-4 DAM AT LAKE GONZALES	21736	1804	14	GB	GB	RT									4			4	4		4	Station added in FY16, flow estimate taken from USGS gage 08169845
GUADALUPE RIVER AT FM 1117 RIVER CROSSING 2.1 MILES SOUTH OF SH 90A 5.2 MILES EAST OF SEGUIN	17134	1804	13	GB	GB	RT									4			4	4		4	Dropped by TCEQ R in FY16
GUADALUPE RIVER IMMEDIATELY DOWNSTREAM OF H-5 DAM AT WOOD LAKE SW OF GONZALES TX	15110	1804	14	GB	GB	RT									4			4	4		4	flow estimate taken from USGS gage 08169845
LAKE DUNLAP-GUADALUPE RIVER NORTH BANK AT ACS PLACE AT MID POINT OF LONE STAR DRIVE	12596	1804	13	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon, flow estimate taken from GBRA Dunlap discharge measurements

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
WEST BANK OF LAKE MCQUEENEY AT LAKE BREEZE SKI LODGE BOAT RAMP 1.20 KILOMETERS UPSTREAM OF FM 78	22189	1804	13	GB	GB	RT									12			12	12		12	Replaced Station 15149 in FY20 - NH3 and TKN will be done bimon, flow estimate taken from GBRA Dunlap discharge measurements
GERONIMO CREEK AT HABERLE ROAD/CR 1103 MILES SOUTH OF GERONIMO	12576	1804A	13	GB	GB	RT									12			12	12		12	ecoregion reference site NH3 and TKN will be done bimonthly
CANYON LAKE SOUTH OF JACOBS CREEK PARK 500 YARDS EAST OF PENINSULA	12598	1805	13	GB	GB	RT									12			12			12	NH3 and TKN will be done bimon
GUADALUPE RIVER 20 METERS UPSTREAM OF FM 1376 AND 2.5 KILOMETERS SOUTH OF SISTERDALE	22082	1806	13	GB	GB	RT									4			4	4		4	Quarterly Routine Station Added in FY19 Due to Elevated E. coli Concentrations Downstream at Station 17404.
GUADALUPE RIVER AT FM 474 AT AMMANS CROSSING NE OF BOERNE	17404	1806	13	GB	GB	RT									4			4	4		4	

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
GUADALUPE RIVER AT FOOTBRIDGE IN LOUISE HAYS PARK APPROX 100M UPSTREAM OF SH16	16244	1806	13	GB	UG	RT												12			12	
GUADALUPE RIVER AT G STREET/FORMERLY OLD MEDINA RD IN KERRVILLE SEGMENT KM 177.9	12616	1806	13	GB	UG	RT								4				4	4		4	VSS removed from conventional in FY22
GUADALUPE RIVER AT HERMANN SONS RD ADJACENT TO HERMANN SONS HOME WEST OF COMFORT	12605	1806	13	GB	UG	RT								4				4	4		4	VSS removed from conventional in FY22, flow estimate taken from USGS gage 8167000
GUADALUPE RIVER AT KERRVILLE STATE PARK SEGMENT KM 174.4	12615	1806	13	GB	UG	RT								4				12	12		12	VSS removed from conventional in FY22, flow estimate taken from USGS gage 8166250
GUADALUPE RIVER AT LOUISE HAYS PARK DAM APPROX 50M DOWNSTREAM OF SH16	16243	1806	13	GB	UG	RT												12			12	
GUADALUPE RIVER AT RIVERVIEW RD IN INGRAM TX	15111	1806	13	GB	UG	RT								4				4	4		4	VSS removed from conventional in FY22

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
GUADALUPE RIVER AT RR 311 1.9 MI SE OF SPRING BRANCH 7.5 MI DOWNSTREAM FROM CURRY CREEK	13700	1806	13	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon
GUADALUPE RIVER AT SAN ANTONIO RD/FM1621 IN WARING	12602	1806	13	GB	UG	RT									4			4	4		4	VSS removed from conventional in FY22, flow estimate taken from USGS gage 8167000
GUADALUPE RIVER AT SH 16 IN KERRVILLE	12617	1806	13	GB	UG	RT												12			12	
GUADALUPE RIVER AT SPLIT ROCK RD OFF SH 27 2.6 KM DOWNSTREAM OF FLATROCK DAM	15113	1806	13	GB	UG	RT									4			4	4		4	VSS removed from conventional in FY22.
GUADALUPE RIVER AT UGRA LAKE DAM	12618	1806	13	GB	UG	RT									4			4	4		4	VSS removed from conventional in FY22
GUADALUPE RIVER CENTER POINT LAKE	12608	1806	13	GB	UG	RT									4			4	4		4	VSS removed from conventionals in FY22, flow estimate taken from USGS gage 8166250

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
HONEY CREEK APPROXIMATELY 1.2 KM UPSTREAM OF CONFLUENCE WITH GUADALUPE RIVER AT UNIMPROVED ROAD CROSSING	15399	1806	13	GB	GB	RT									4			4	4		4	Routine Quarterly Monitoring Added for FY21
CAMP MEETING CREEK 0.1 KM UPSTREAM CONFLUENCE WITH GUADALUPE IN KERRVILLE	12546	1806A	13	GB	UG	RT									4			12	12		12	Monthly bacteria, flow, field added in FY22 VSS removed from conventional in FY22
QUINLAN CREEK AT TRAVIS STREET IN KERRVILLE	12541	1806D	13	GB	UG	RT												12	12		12	
TOWN CREEK AT HAMILTON STREET IN KERRVILLE	12549	1806E	13	GB	UG	RT												12	12		12	
COLETO CREEK RESERVOIR AT MID POINT OF DAM ON COLETO CREEK PARK ROAD	20827	1807	14	GB	GB	RT									12			12			12	depth profiles will be completed quarterly; nh3 and tkn bimonthly
LOWER SAN MARCOS RIVER AT SH 80 SOUTH OF LULING	12626	1808	11	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon
SAN MARCOS RIVER AT US90A 3.3KM WEST OF INTERSECTION OF US90A AND US183 IN GONZALES 7KM UPSTREAM OF CONFL. WITH GUADALUPE RIVER	16578	1808	14	GB	GB	RT									4			4	4		4	flow estimate taken from USGS gage 8172000

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
PLUM CREEK AT CR 202 SE OF LOCKHART	12647	1810	11	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon, flow estimate taken from USGS gage 8172400
PLUM CREEK AT OLD WOODEN BRIDGE ON CALDWELL CR 135 SE OF LULING	12640	1810	11	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon, flow estimate taken from USGS gage 8173000
PLUM CREEK AT PLUM CREEK ROAD NORTH OF UHLAND	17406	1810	11	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon
COMAL RIVER AT LANDA PARK AREA 16 2.45 MI UPSTREAM FROM CONFLUENCE WITH GUADALUPE RIVER IN NEW BRAUNFELS	15082	1811	13	GB	GB	RT									12			12	12		12	TKN and NH3 done bimonthly
COMAL RIVER DOWNSTREAM CLEMONS DAM IN NEW BRAUNFELS	12653	1811	13	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon
DRY COMAL CREEK AT MISSOURI-KANSAS-TEXAS RAILROAD CROSSING IN NEW BRAUNFELS	12570	1811A	13	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon
GUADALUPE RIVER AT RIVER RD 2ND CROSSING UPSTREAM OF NEW BRAUNFELS	12658	1812	13	GB	GB	RT									12			12	12		12	NH3 and TKN will be done bimon, flow estimate taken from USGS gage 8167800

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
GUADALUPE RIVER AT THE BEGINNING OF CYPRESS BEND PARK IN NEW BRAUNFELS	12656	1812	13	GB	GB	RT									4			4	4		4	
BLANCO RIVER AT BLANCO STATE PARK PR 23	12669	1813	11	GB	HZ	RT									8			8	8		8	conventionals-Total P, NO3-N, NH3-N, TSS &; TKN
BLANCO RIVER IMMEDIATELY UPSTREAM OF RIVER RUN AND PANY DR 0.3 MI EAST OF RR 1623 AT HINES BRANCH IN BLANCO	17528	1813	11	GB	HZ	RT									8			8	8		8	conventionals-Total P, NO3-N, NH3-N, TSS &; TKN. HZ to sample during months when FO does not complete quarterly sampling, flow estimate taken from LCRA flow gage 7817
BLANCO RIVER AT BRIDGE ON SH 12 AT WIMBERLEY	12661	1813	11	GB	HZ	RT									4			4	4		4	conventionals-Total P, NO3-N, NH3-N, TSS &; TKN
BLANCO RIVER AT FM 165 1/2 MILE EAST OF BLANCO	12668	1813	11	GB	HZ	RT									8			8	8		8	conventionals-Total P, NO3-N, NH3-N, TSS &; TKN.

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
BLANCO RIVER AT LOW WATER CROSSING AT CR 174/FULTON RANCH RD	12660	1813	11	GB	HZ	RT									4			4	4		4	conventionals-Total P, NO3-N, NH3-N, TSS, & TKN
BLANCO RIVER AT LOW WATER CROSSING CR1492 AT PIONEER TOWN	12663	1813	11	GB	HZ	RT									4			4	4		4	conventionals-Total P, NO3-N, NH3-N, TSS
BLANCO RIVER AT PLEASANT VALLEY CROSSING ON FISHER STORE RD	12665	1813	11	GB	HZ	RT									4			4	4		4	conventionals-Total P, NO3-N, NH3-N, TSS
UPPER SAN MARCOS RIVER IMMEDIATELY UPSTREAM OF IH 35 BRIDGE AT SAN MARCOS	12672	1814	11	GB	GB	RT									4			4	4		4	
CYPRESS CREEK AT CAMP YOUNG JUDAEA 830 METERS DOWNSTREAM OF JACOBS WELLS ROAD IN THE CITY OF WOODCREEK IN HAYS COUNTY	22109	1815	11	GB	TI	RT									4			4	4		4	Conventionals-Total P, NO3-N, NH3-N, TSS, flow estimate taken from USGS gage 08170990
CYPRESS CREEK AT CONFLUENCE WITH THE BLANCO RIVER	12673	1815	11	GB	TI	BS	2												2			24 Hour DO & Streamflow CRP Monitoring
CYPRESS CREEK AT CONFLUENCE WITH THE BLANCO RIVER	12673	1815	11	GB	TI	RT									4			4	4		4	Conventionals-Total P, NO3-N, NH3-N, TSS

Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
CYPRESS CREEK AT DOWNSTREAM END IN BLUE HOLE CAMPGROUND	12675	1815	11	GB	TI	BS	2											2				24 Hour DO & Streamflow CRP Monitoring
CYPRESS CREEK AT DOWNSTREAM END IN BLUE HOLE CAMPGROUND	12675	1815	11	GB	TI	RT								4			4	4		4		Conventionals-Total P, NO3-N, NH3-N, TSS
CYPRESS CREEK AT FM 12 AT WIMBERLEY	12674	1815	11	GB	GB	RT								4			4	4		4		
CYPRESS CREEK AT JACOBS WELL SPRING APPROXIMATELY 670 METERS UPSTREAM OF HAYS CR 220/JACOBS WELL ROAD NORTH OF WIMBERLEY CAMS 0745	12677	1815	11	GB	TI	RT								4			4	4		4		Conventionals-Total P, NO3-N, NH3-N, TSS
CYPRESS CREEK AT RR 12 1 MILE NORTH OF WIMBERLEY	12676	1815	11	GB	TI	RT								4			4	4		4		Conventionals-Total P, NO3-N, NH3-N, TSS
CYPRESS CREEK AT WOODCREEK DRIVE DAM IN HAYS COUNTY	22110	1815	11	GB	TI	RT								4			4	4		4		Conventionals-Total P, NO3-N, NH3-N, TSS, flow estimate taken from USGS gage 08170990


Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
JOHNSON CREEK AT SH 39 IN INGRAM	12678	1816	13	GB	GB	BS		1	1	1											1	ALM postponed in FY25 due to flooding. One ALM to be completed in critical period FY26
JOHNSON CREEK AT SH 39 IN INGRAM	12678	1816	13	GB	UG	BS	1											1				24 hour DO, and flow in support of ALM
JOHNSON CREEK AT SH 39 IN INGRAM	12678	1816	13	GB	UG	RT								4			4	4			4	VSS removed from conventional in FY22. NH3 added for FY26/27.
NORTH FORK GUADALUPE RIVER AT FM 1340	12681	1817	13	GB	GB	BS		2	2	2											2	FY26 ALM
NORTH FORK GUADALUPE RIVER AT FM 1340	12681	1817	13	GB	UG	BS	2							2				2				24 hour DO, conventionals, and flow in support of ALM
NORTH FORK GUADALUPE AT RIVER GAGING STATION NEAR CAMP WALDEMAR	12682	1817	13	GB	UG	RT								4			4	4			4	NH3 removed FY24


Site Description	Station ID	Waterbody ID	Region	SE	CE	MT	24 hr DO	AqHab	Benthics	Nekton	Metal Water	Organic Water	Metal Sed	Organic Sed	Conv	Amb Tox Water	Amb Tox Sed	Bacteria	Flow	Fish Tissue	Field	Comments
SOUTH FORK GUADALUPE ADJACENT TO HUNT LIONS PARK	12684	1818	13	GB	UG	RT								4			4	4			4	
SAN ANTONIO RIVER FM 2506 EAST OF FANNIN	12790	1901	14	GB	GB	RT								12			12	12			12	NH3 and TKN will be done bimonthly, flow estimate taken from USGS gage 08188500

Appendix C: Station Location Maps

Station Location Maps

Maps of stations monitored by GBRA are provided below. The maps were generated by GBRA. This product is for informational purposes and may not have been prepared for or be suitable for legal, engineering, or surveying purposes. It does not represent an on-the-ground survey and represents only the approximate relative location of property boundaries. For more information concerning this map, contact the contact the PM at 830-379-5822.

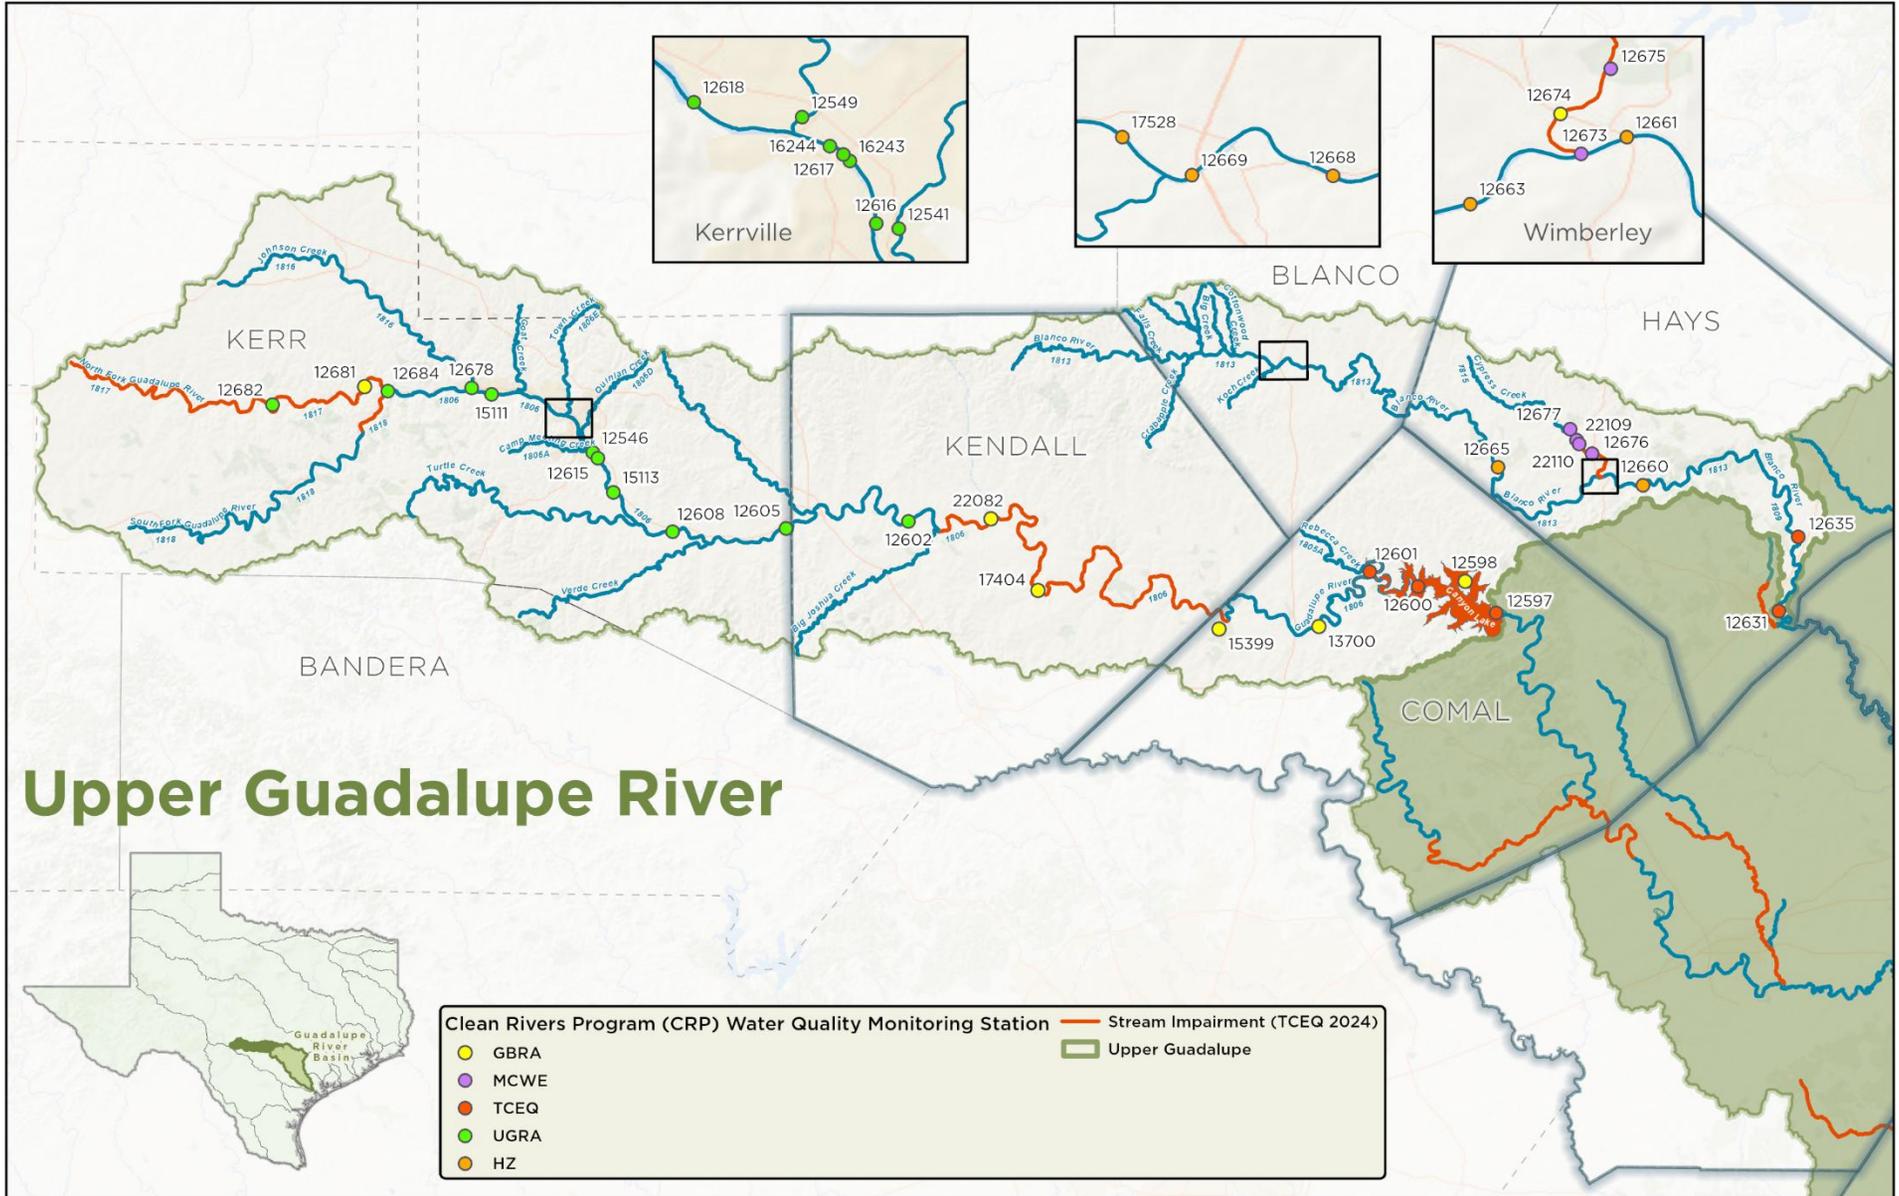


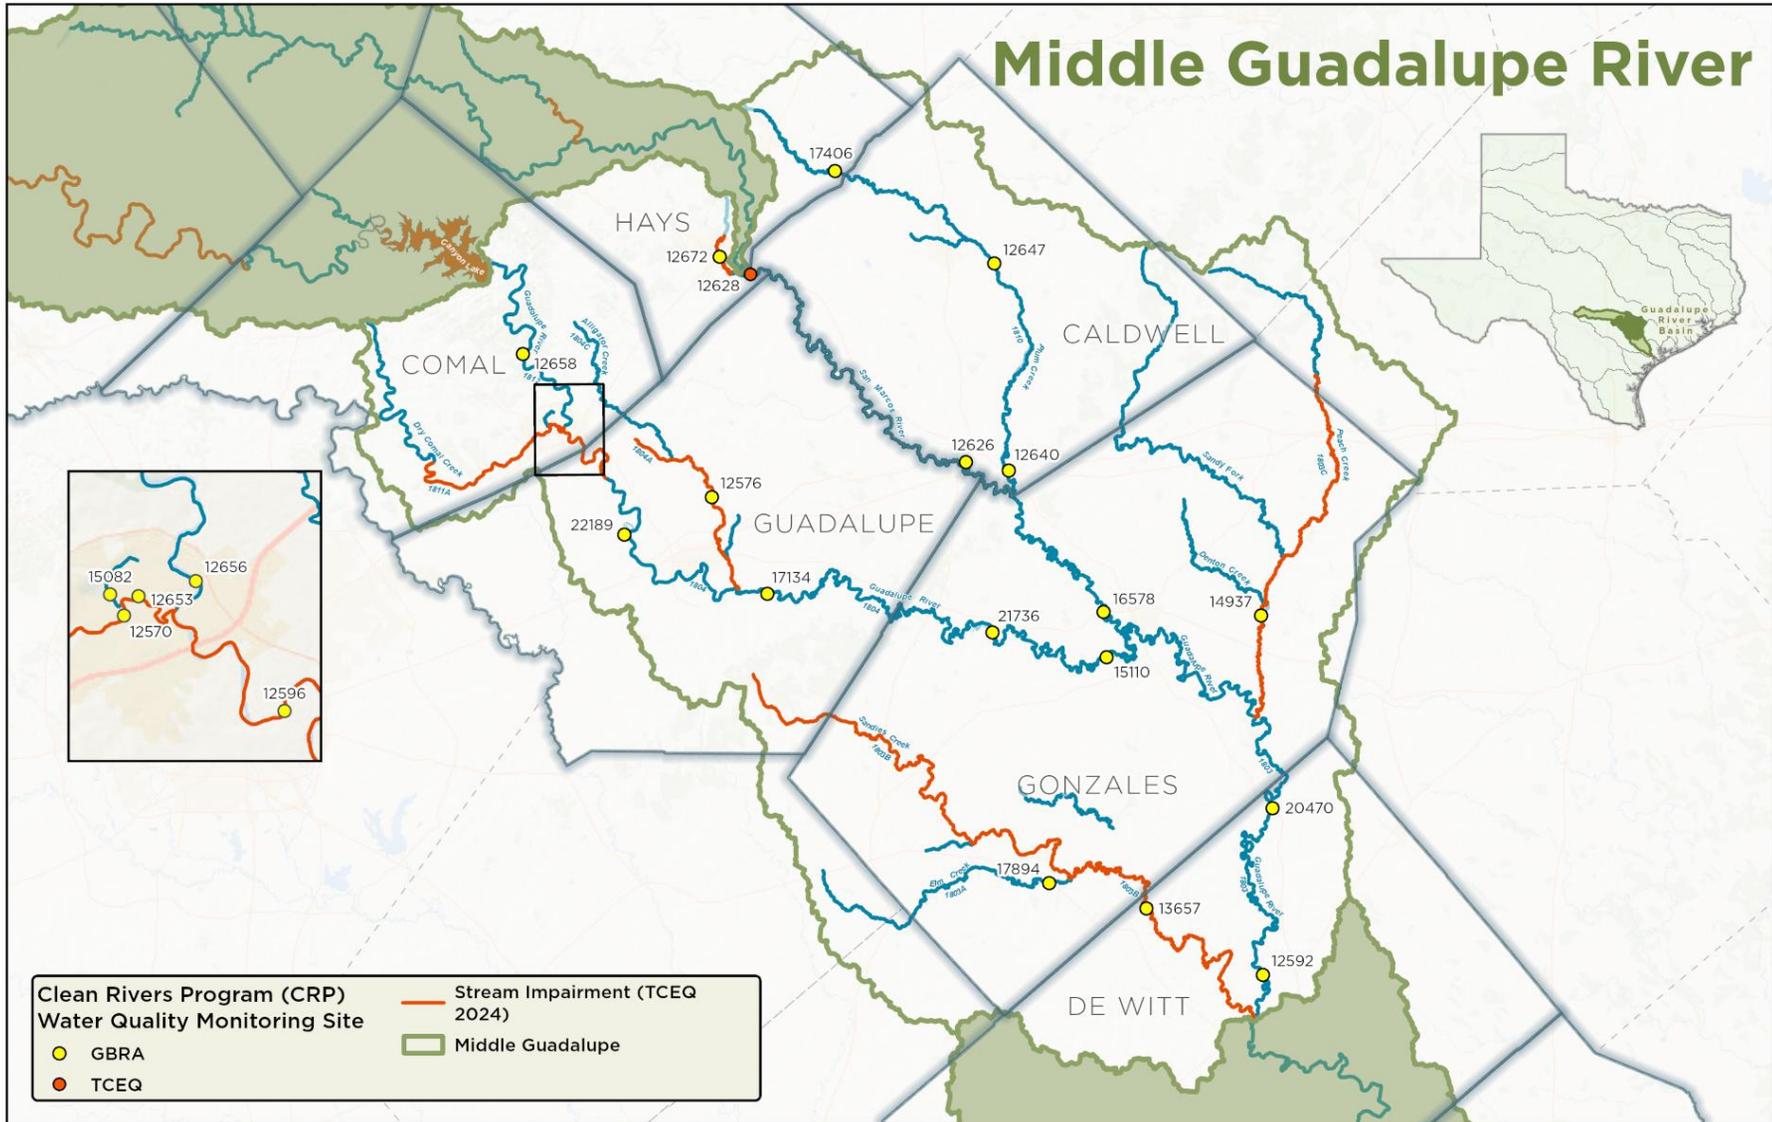

Lower Guadalupe River

Clean Rivers Program (CRP) Water Quality Monitoring Site

- GBRA
- TCEQ
- Stream Impairment (TCEQ 2024)
- ▭ Lower Guadalupe

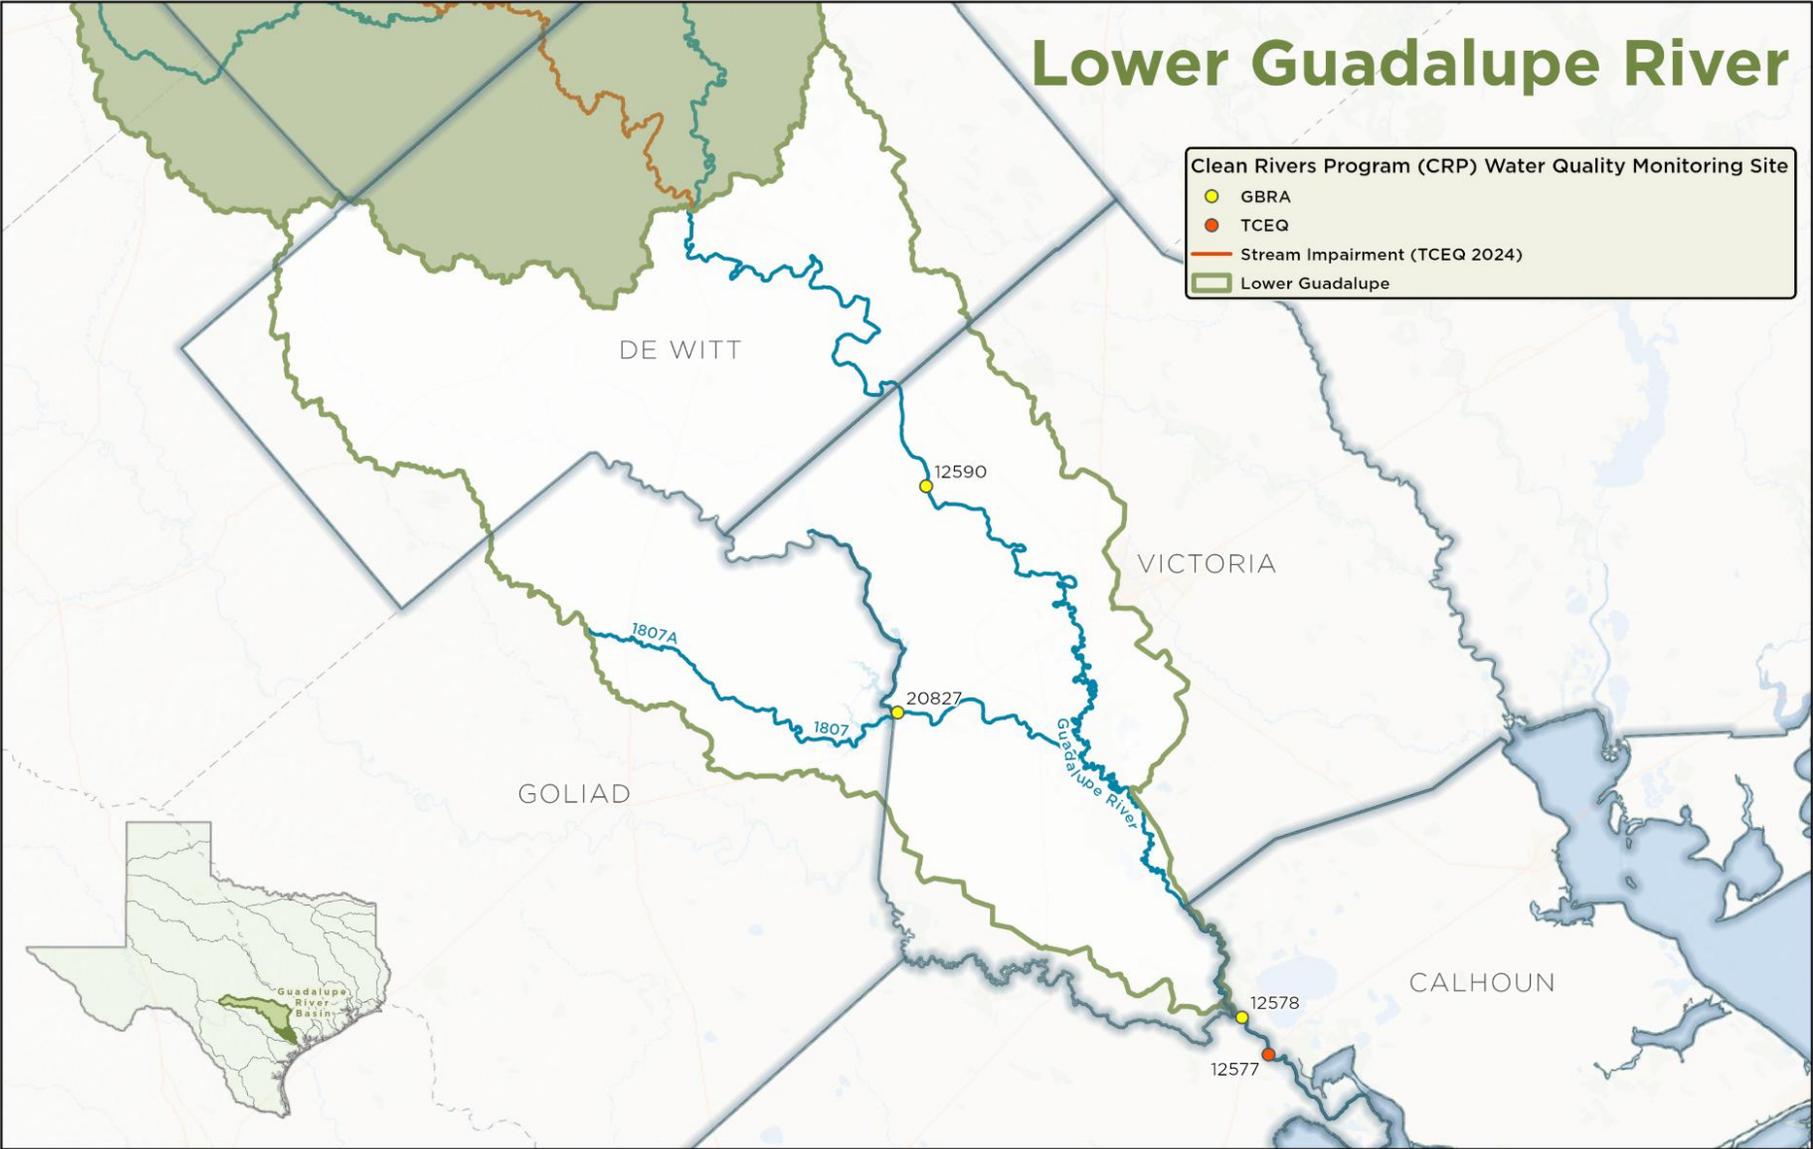

Appendix D: Field Data Sheets

GBRA Field Data Reporting Form in PDF and backup Hard copy Version

Texas Commission on Environmental Quality
Surface Water Quality Monitoring Program

GBRA Field Data Reporting Form

RTAG#				REGION		EMAIL-ID:			
STATION ID		SEGMENT		SEQUENCE		COLLECTOR			
STATION ID		SEGMENT		SEQUENCE		DATA SOURCE			

Station Description _____

GRAB SAMPLE							
M	M	D	D	Y	Y	Y	Y
DATE							
H	H	M	M	x			
TIME				DEPTH		M - meters F - feet	

COMPOSITE CATEGORY:		T - TIME	S - SPACE (I.e. Depth)	B - BOTH	F - FLOW WEIGHT		
M	M	D	D	Y	Y	Y	Y
START DATE							
H	H	M	M	START DEPTH (SURFACE)		M - Meters F - Feet	
START TIME				END DEPTH (DEEPEST)		M - Meters F - Feet	
M	M	D	D	Y	Y	Y	Y
END DATE							
H	H	M	M	END TIME			
END TIME							
COMPOSITE TYPE:		## - Number of Grabs in Composite			CN - Continuous		

00010	WATER TEMP (*C only)	72053	DAYS SINCE LAST SIGNIFICANT PRECIPITATION
00400	pH (s.u)	01351	FLOW SEVERITY
00300	D.O. (mg/L)		1-no flow 2-low
00094	SPECIFIC COND (umhos/cm)		3-normal 5-high 4-flood 6-dry
00480	SALINITY (ppt, marine only)	00061	INSTANTANEOUS STREAM FLOW (ft ³ /sec)
00078	TRANSPARENCY, SECCHI (meters)	89835	FLOW MEASUREMENT METHOD
			1- Flow Gage Station 2- Electric
			3- Mechanical 4- Weir/Flume
			5-Acoustic Doppler
00051	RESERVOIR ACCESS NOT POSSIBLE LEVEL TOO LOW (ENTER 1 IF REPORTING)*	74069	FLOW ESTIMATE (ft ³ /sec)
00052	RESERVOIR STAGE (feet above mean sea level)*	82903	DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE (meters)*
00053	RESERVOIR PERCENT FULL (%)*	89864	MAXIMUM POOL WIDTH AT TIME OF STUDY (meters)*
		89865	MAXIMUM POOL DEPTH AT TIME OF STUDY(meters)
		89869	POOL LENGTH (meters) *
		89870	% POOL COVERAGE IN 500 M REACH (%) *

*Parameters related to data collection in perennial pools; i.e., Flow Severity of 1 and Flow of 0 cfs reported.

Measurement Comments and Field Observations:

GBRA's Field Data Reporting Form in Excel form

GBRA Field Data Reporting Form

LIMS Sample ID(s):												COLLECTOR (First Initial & Last Name)												
STATION ID				SEGMENT				REGION				DATA SOURCE												
Station Description																								
GRAB SAMPLE																								
M M D D Y Y Y Y												H H M M				M = Meters								
Date												Time				DEPTH				F = Feet				
COMPOSITE SAMPLE																								
T		COMPOSITE CATEGOF T = TIME						S = SPACE				B = BOTH				F = FLOW WEIGHT								
M M D D Y Y Y Y												H H M M				START DEPTH				M = Meters				
START DATE												START TIME				F = Feet				M				
M M D D Y Y Y Y												H H M M				END DEPTH				M = Meters				
END DATE												END TIME				(DEEPEST)				F = Feet				
24		COMPOSITE TYPE:						## = Number of Grabs in Composite				CN = Continuous												
00010		WATER TEMP (°C only)										72053	Days Since Last Significant Precipitation											
00400		pH (s. u.)											FLOW SEVERITY				1-no flow 2-low							
00300		D. O. (mg/L)										01351	3-normal		5-high		4-flood		6-dry					
00094		SPECIFIC COND (µmhos/cm)										00061	INSTANTANEOUS STREAM FLOW (ft ³ /sec)											
00480		SALINITY (ppt, marine only)											FLOW MEASUREMENT METHOD											
00078		Transparency, SECCHI (meters)											1-FlowGage Station				2-Electric							
		RESERVOIR ACCESS NOT POSSIBLE (Enter 1 if Reporting)*										89835	3-Mechanical				4-Wier/Flume							
												74069	5-Doppler											
		RESERVOIR STAGE (feet above mean sea level)*										82903	FLOW ESTIMATE (ft ³ /sec)											
00052		RESERVOIR PERCENT FULL										89864	DEPTH OF BOTTOM AT SAMPLE SITE (feet)											
												89865	MAXIMUM POOL WIDTH (meters)*											
												89869	MAXIMUM POOL DEPTH (meters)*											
												89870	POOL LENGTH (meters)*											
													% POOL COVERAGE IN 500 Meter REACH											
*Parameters related to data collection in perennial pools; i.e., Flow Severity of 1 and Flow of 0 cfs reported.																								
Measurement Comments and Field Observations:																								
TCEQ-20154 (Rev. 05/14/2004) GBRA Revision 2 (07-30-18)												Page 1 of 1												

UGRA Field Data Reporting Form

UGRA Field Data Reporting Form

RTAG#				REGION		EMAIL-ID:			
STATION ID		SEGMENT		SEQUENCE		COLLECTOR			
						DATA SOURCE			

Station Description _____

GRAB SAMPLE														
M	M	D	D	Y	Y	Y	Y	H	H	M	M	DEPTH		M = meters F = feet
DATE										TIME				
COMPOSITE SAMPLE														
COMPOSITE CATEGORY:		T = TIME			S = SPACE (i.e. Depth)			B = BOTH		F = FLOW WEIGHT				
M	M	D	D	Y	Y	Y	Y	H	H	M	M	START DEPTH		M = Meters
START DATE										START TIME		(SURFACE)		F = Feet
M	M	D	D	Y	Y	Y	Y	H	H	M	M	END DEPTH		M = Meters
END DATE										END TIME		(DEEPEST)		F = Feet
COMPOSITE TYPE:		# = Number of Grabs in Composite					CN = Continuous							

00010	WATER TEMP (°C only)	72053	DAYS SINCE LAST SIGNIFICANT PRECIPITATION			
00300	D.O. (mg/L)	01351	FLOW SEVERITY			
00094	SPECIFIC COND (µmhos/cm)		1-no flow	2-low		
00400	pH (s.u)		3-normal	5-high	4-flood	6-dry
		00061	INSTANTANEOUS STREAM FLOW (ft ³ /sec)			
		89835	FLOW MEASUREMENT METHOD			
00078	Transparency, Secchi (meters)		1- Flow Gage Station	2- Electric		
			3- Mechanical	4- Weir/Flume		
			5-Doppler			
			74069	FLOW ESTIMATE (ft ³ /sec)		
		89864	MAXIMUM POOL WIDTH (meters) *			
		89869	POOL LENGTH (meters) *			
		89865	MAXIMUM POOL DEPTH (meters) *			
		82903	DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE (meters) *			
		89870	PERCENT POOL COVERAGE IN 500 METER REACH			

*Parameters related to data collection in perennial pools; i.e., Flow Severity of 1 and Flow of zero reported.

Measurement Comments and Field Observations:

HZ Field Data Reporting Form PDF and backup Hard Copy version

Texas Commission on Environmental Quality
 Surface Water Quality Monitoring Program
HZ Field Data Reporting Form

RTAG# _____ REGION _____ EMAIL-ID: LG JB _____ COLLECTOR _____

STATION ID _____ SEGMENT _____ SEQUENCE _____ DATA SOURCE _____

Station Description _____

GRAB SAMPLE

DATE: M M D D Y Y Y Y TIME: H H M M DEPTH: 0 3 M = meters F = feet

COMPOSITE SAMPLE

COMPOSITE CATEGORY: T = TIME S = SPACE (i.e. Depth) B = BOTH F = FLOW WEIGHT

START DATE: M M D D Y Y Y Y START TIME: H H M M START DEPTH (SURFACE): M = Meters F = Feet

END DATE: M M D D Y Y Y Y END TIME: H H M M END DEPTH (DEEPEST): M = Meters F = Feet

COMPOSITE TYPE: ## = Number of Grabs in Composite CN = Continuous

00010	WATER TEMP (°C only)	72053	DAYS SINCE LAST SIGNIFICANT PRECIPITATION
00400	pH (s.u)	01351	FLOW SEVERITY
00300	D.O. (mg/L)		3-normal 5-high 1-no flow 2-low
00064	SPECIFIC COND (µmhos/cm)	00061	INSTANTANEOUS STREAM FLOW (ft ³ /sec)
00480	SALINITY (ppt, marine only)	89835	FLOW MEASUREMENT METHOD
89978	PRIMARY CONTACT, OBSERVED ACTIVITY (# of people observed)		1- Flow Gage Station 2- Electric 3- Mechanical 4- Weir/Fume 5-Acoustic Doppler
89979	EVIDENCE OF PRIMARY CONTACT RECREATION (1 = OBSERVED, 0 = NOT OBSERVED)	74069	FLOW ESTIMATE (ft ³ /sec)
00051	RESERVOIR ACCESS NOT POSSIBLE LEVEL TOO LOW (ENTER 1 IF REPORTING)*	82903	DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE (meters)*
00052	RESERVOIR STAGE (feet above mean sea level)*	89864	MAXIMUM POOL WIDTH AT TIME OF STUDY (meters)*
00053	RESERVOIR PERCENT FULL (%)*	89885	MAXIMUM POOL DEPTH AT TIME OF STUDY(meters)
		89869	POOL LENGTH (meters) *
		89870	% POOL COVERAGE IN 500 M REACH (%) *

*Parameters related to data collection in perennial pools; i.e., Flow Severity of 1 and Flow of 0 cfs reported.

Measurement Comments and Field Observations:

HZ Field Data Reporting Form

LIMS Sample ID(s):		COLLECTOR (First Initial & Last Name)					
STATION ID	SEGMENT	REGION	DATA SOURCE				
Station Description							

GRAB SAMPLE						
Date		Time		DEPTH		F = Feet
M M	D D	Y Y	Y Y	H H	M M	M = Meters

COMPOSITE SAMPLE						
T	COMPOSITE CATEGOF T = TIME		S = SPACE	B = BOTH	F = FLOW WEIGHT	
START DATE		START TIME		START DEPTH		M = Meters
M M	D D	Y Y	Y Y	H H	M M	F = Feet
END DATE		END TIME		END DEPTH (DEEPEST)		M = Meters
M M	D D	Y Y	Y Y	H H	M M	F = Feet
24	COMPOSITE TYPE:		## = Number of Grabs in Composite		CN = Continuous	

00010	WATER TEMP (°C only)	72053	Days Since Last Significant Precipitation			
00400	pH (s. u.)		FLOW SEVERITY	1-no flow	2-low	
00300	D. O. (mg/L)	01351		3-normal	5-high	4-flood 6-dry
00094	SPECIFIC COND (µmhos/cm)	00061	INSTANTANEOUS STREAM FLOW (ft ³ /sec)			
00480	SALINITY (ppt, marine only)		FLOW MEASUREMENT METHOD			
00078	Transparency, SECCHI (meter)	89835	1-FlowGage Station	2-Electric		
	RESERVOIR ACCESS NOT POSSIBLE (Enter 1 if Reporting)*	74069	3-Mechanical	4-Weir/Flume		
00051		82903	5-Doppler			
	RESERVOIR STAGE (feet above mean sea level)*	89864	FLOW ESTIMATE (ft ³ /sec)			
00052		89865	DEPTH OF BOTTOM AT SAMPLE SITE (feet)			
00053	RESERVOIR PERCENT FULL	89869	MAXIMUM POOL WIDTH (meters)*			
		89870	MAXIMUM POOL DEPTH (meters)*			
			POOL LENGTH (meters)*			
			% POOL COVERAGE IN 500 Meter REACH			

*Parameters related to data collection in perennial pools; i.e., Flow Severity of 1 and Flow of 0 cfs reported.

Measurement Comments and Field Observations:

TCEQ-20154 (Rev. 05/14/2004) GBRA Revision 2 (07-30-18)

Page 1 of 1

MCWE Field Data Reporting Form in PDF and Back up Hard Copy Version

Texas Commission on Environmental Quality
 Surface Water Quality Monitoring Program
 MCWE Field Data Reporting Form

RTAG# _____ REGION _____ EMAIL-ID: LG JB _____ COLLECTOR _____
 STATION ID _____ SEGMENT _____ SEQUENCE _____ DATA SOURCE _____

Station Description _____

GRAB SAMPLE
 DATE: M M D D Y Y Y Y TIME: H H M M DEPTH: 0 3 M Meters F = feet

COMPOSITE SAMPLE
 S = SPACE (i.e. Depth) B = BOTH F = FLOW WEIGHT
 COMPOSITE CATEGORY: T = TIME
 START DATE: M M D D Y Y Y Y START TIME: H H M M START DEPTH (SURFACE): M Meters F = Feet
 END DATE: M M D D Y Y Y Y END TIME: H H M M END DEPTH (DEEPEST): M Meters F = Feet
 COMPOSITE TYPE: ## = Number of Grabs in Composite CN = Continuous

00010	WATER TEMP (°C only)	72053	DAYS SINCE LAST SIGNIFICANT PRECIPITATION	
00400	pH (s.u)	01351	FLOW SEVERITY	1-no flow 2-low
00300	D.O. (mg/L)		3-normal 5-high 4-flood 6-dry	
00084	SPECIFIC COND (µmhos/cm)	00081	INSTANTANEOUS STREAM FLOW (ft ³ /sec)	
00480	SALINITY (ppt, marine only)	89835	FLOW MEASUREMENT METHOD 1- Flow Gage Station 2- Electric 3- Mechanical 4- Weir/Flume 5-Acoustic Doppler	
89978	PRIMARY CONTACT, OBSERVED ACTIVITY (# of people observed)	74089	FLOW ESTIMATE (ft ³ /sec)	
89979	EVIDENCE OF PRIMARY CONTACT RECREATION (1 = OBSERVED, 0 = NOT OBSERVED)	82903	DEPTH OF BOTTOM OF WATER BODY AT SAMPLE SITE (meters)*	
00051	RESERVOIR ACCESS NOT POSSIBLE LEVEL TOO LOW (ENTER 1 IF REPORTING)*	89884	MAXIMUM POOL WIDTH AT TIME OF STUDY (meters)*	
00052	RESERVOIR STAGE (feet above mean sea level)*	89885	MAXIMUM POOL DEPTH AT TIME OF STUDY(meters)	
00053	RESERVOIR PERCENT FULL (%)*	89889	POOL LENGTH (meters) *	
		89870	% POOL COVERAGE IN 500 M REACH (%)*	

*Parameters related to data collection in perennial pools; i.e., Flow Severity of 1 and Flow of 0 cfs reported.

Measurement Comments and Field Observations:

Print



Save As...

Regional Environmental Laboratory CHAIN OF CUSTODY



600 E. Euclid
San Antonio, TX 78212
Phone: (210) 302-3649
FAX (210) 302-3694

Report To: _____	Phone #: _____	Collector's Name: _____
Address: _____	FAX #: _____	Field Comments: _____
City, State, ZIP: _____	E-mail: _____	_____
Rush Analysis (Additional Fees Apply) <input type="checkbox"/> 3-7 days	Report Delivery: <input type="checkbox"/> Mail <input type="checkbox"/> Fax <input type="checkbox"/> E-mail	Method of Shipment: <input type="checkbox"/> Hand Delivered <input type="checkbox"/> Mailed <input type="checkbox"/> Ice

Sample #	Sample Location	1.	2.	3.	4.	Collection Date/Time	Requested Analyses					5.	6.	Container Lot Number (Microbiology Only)	Lab Use ONLY	
		Collection Method	Sample Type	Matrix	Composite Start Date/Time							Container Type	Type of Preservation		Therm. ID: C01-_____ Receipt Temp. (°C) Observed/Corrected ____/____ pH <2 Y or N pH Paper: _____	

Relinquished by: _____	Date/Time: _____	Received by: _____	Date/Time: _____
Relinquished by: _____	Date/Time: _____	Received by: _____	Date/Time: _____
Relinquished by: _____	Date/Time: _____	Received by: _____	Date/Time: _____
Relinquished by: _____	Date/Time: _____	Received by: _____	Date/Time: _____
Lab Comments: _____ NA - Not Applicable			
1. Collection Method: G - Grab C - Composite	2. Sample Type: EF - Effluent, IF - Influent, SW - Surfacewater, ST - Stormwater, GW - Groundwater, QC - Quality Control, O - Other (Specify in Comments)	3. Matrix: NPW - Non-Potable Water, SE - Sediment, SO - Soil, O - Other (Specify in Comments)	4. Composite Samples require Composite Start Date/Time and Collection Date/Time
		5. Container Type: GC - Gallon Cubitainer, QC - Quart Cubitainer, AB - Amber Glass Bottle, CB - Clear Glass Bottle, PB - Plastic Bottle, AP - Amber Plastic, WP - Whirl-pak	6. Type of Preservation: U - Unpreserved (No Chemical Preservation), S - Sulfuric Acid, H - Hydrochloric Acid, N - Nitric Acid, P - Phosphoric Acid, O - Other (Specify in Comments)

Appendix F: Data Review Checklist and Summary Shells

Data Review Checklist

This checklist is to be used by the Planning Agency and other entities handling the monitoring data in order to review data before submitting to the TCEQ. This table may not contain all of the data review tasks being conducted.

Data Format and Structure	Y, N, or N/A
Are there any duplicate Tag Id numbers in the Events file?	
Do the Tag prefixes correctly represent the entity providing the data?	
Have any Tag Id numbers been used in previous data submissions?	
Are Tag IDs associated with a valid SLOC?	
Are sampling Dates in the correct format, MM/DD/YYYY with leading zeros?	
Are sampling Times based on the 24 hr clock (e.g. 09:04) with leading zeros?	
Is the Comments field filled in where appropriate (e.g. unusual occurrence, sampling problems, unrepresentative of ambient water quality)?	
Are Submitting Entity, Collecting Entity, and Monitoring Type codes used correctly?	
Do sampling dates in the Results file match those in the Events file for each Tag Id?	
Are values represented by a valid parameter code with the correct units?	
Are there any duplicate parameter codes for the same Tag Id?	
Are there any invalid symbols in the Greater Than/Less Than (GT/LT) field?	
Are there any Tag Ids in the Results file that are not in the Events file or vice versa?	
Data Quality Review	Y, N, or N/A
Are "less-than" values reported at the LOQ? If no, explain in Data Summary.	
Have the outliers been verified and a "1" placed in the Verify_flg field?	
Have checks on correctness of analysis or data reasonableness been performed? e.g., Is ortho-phosphorus less than total phosphorus? Are dissolved metal concentrations less than or equal to total metals? Is the minimum 24 hour DO less than the maximum 24 hour DO? Do the values appear to be consistent with what is expected for site?	
Have at least 10% of the data in the data set been reviewed against the field and laboratory data sheets?	
Are all parameter codes in the data set listed in the QAPP?	
Are all stations in the data set listed in the QAPP?	
Documentation Review	Y, N, or N/A
Are blank results acceptable as specified in the QAPP?	
Were control charts used to determine the acceptability of lab duplicates (if applicable)?	
Was documentation of any unusual occurrences that may affect water quality included in the Event file's Comments field?	
Were there any failures in sampling methods and/or deviations from sample design requirements that resulted in unreportable data? If yes, explain in Data Summary.	
Were there any failures in field and/or laboratory measurement systems that were not resolvable and resulted in unreportable data? If yes, explain in Data Summary.	
Was the laboratory's NELAP Accreditation current for analysis conducted?	
Did participants follow the requirements of this QAPP in the collection, analysis, and reporting of data?	

Data Summary

Data Set Information

Data Source: _____

Date Submitted: _____

Tag_id Range: _____

Date Range: _____

- I certify that all data in this data set meets the requirements specified in Texas Water Code Chapter 5, Subchapter R (TWC §5.801 et seq) and Title 30 Texas Administrative Code Chapter 25, Subchapters A & B.
- This data set has been reviewed using the criteria in the Data Review Checklist.

Planning Agency Data Manager: _____ Date: _____

Please explain in the table below any data discrepancies discovered during data review including:

- Inconsistencies with LOQs
- Failures in sampling methods and/or laboratory procedures that resulted in data that could not be reported to the TCEQ (indicate items for which the Corrective Action Process has been initiated and send *Corrective Action Status Report* with the applicable Progress Report).

Dataset ____ contains data from FY__ QAPP Submitting Entity code __ and collecting entity __. This is field and lab data that was collected by the (collecting entity). Analyses were performed by the (lab name). The following tables explain discrepancies or missing data as well as calculated data loss.

Discrepancies or missing data for the listed tag ID:

Tag ID	Station ID	Date	Parameters	Type of Problem	Comment/PreCAPs/CAPs

Data Loss

Parameter	Missing Data points out of Total	Percent Data Loss for this Dataset	Parameter	Missing Data points out of Total	Percent Data Loss for this Dataset

Appendix G: Biological Monitoring Electronic Field Sheet

Stream Physical Characteristics Sheet

Stream Physical Characteristics - Transect 1										Page	1	of	6		
Date:		TCEQ Site#			State Name:										
Transect Coordinates:		N	Stream Width (m)			Channel Flow Status:									
(At Center of Transect)		W													
LB Natural Buffer (m)		Tree Canopy Cover (%)					RB Natural Buffer(m)								
		LB	CL	CR	RB										
LB Slope (°)		LB Erosion Potential (%)			RB Slope (°)		RB Erosion Potential (%)								
LB Riparian Vegetaton Types (%)					RB Riparian Vegetation Types (%)										
LB Trees	LB Shrubs	LB Grasses & Forbes			RB Trees	RB Shrubs	RB Grasses & Forbes								
LB Cultivated Fields		LB Other			RB Cultivated Fields			RB Other							
Stream Depths (at points across transect) (m)										Thalweg (m)					
										Average Depth (m)					
Habitat Type		Dominant Substrate Type			Substrate Gravel or Larger (%)										
Instream Cover (%)		Macrophyte Abundance			Algae Abundance		# of Cover Types								
Instream Cover Types:		<input type="checkbox"/> Large Woody Debris			<input type="checkbox"/> Small Woody Debris										
<input type="checkbox"/> Gravel	<input type="checkbox"/> Cobble	<input type="checkbox"/> Leaf Packs	<input type="checkbox"/> Root Wads	<input type="checkbox"/> Overhanging Vegetation											
<input type="checkbox"/> Boulder	<input type="checkbox"/> Undercut Bank	<input type="checkbox"/> Artificial Cover		<input type="checkbox"/> Macrophytes											
<input type="checkbox"/> Algae	<input type="checkbox"/> Other1:	<input type="checkbox"/> Other2:	<input type="checkbox"/> Other3:												
Notes															